

Online Water-Soluble Iron Speciation in Ambient Aerosols under Cloud-Water Relevant and Neutral Conditions

Sabine Luechtrath¹, Sven Klemer¹, Florian Fröhlich¹, Darius Ceburnis², Dominik van Pinxteren³, Hartmut Herrmann³, Wolfgang Frenzel¹, Andreas Held¹

5 ¹ Chair of Environmental Chemistry and Air Research, Technische Universität Berlin, Berlin, 10623, Germany

² The Ryan Institute's Centre for Climate & Air Pollution Studies (C-CAPS), University of Galway, Galway, H91 CF50, Republic of Ireland

³ Leibniz Institute for Tropospheric Research (TROPOS), Atmospheric Chemistry Department (ACD), 04318 Leipzig, Germany.

10 *Correspondence to:* sabine.luechtrath@tu-berlin.de

Abstract. We present the first online instrument for the speciation of water-soluble iron in ambient aerosols under cloud-water relevant and neutral conditions, enabling simultaneous quantification of Fe(II) (ws-Fe(II)) and total water-soluble Fe (total ws-Fe). The system combines flow injection analysis with spectrophotometric detection of the Fe(II)–ferrozine complex using a liquid waveguide capillary cell (LWCC) for sensitive detection thus providing time-resolved measurements of iron solubility with high temporal resolution and good reproducibility. The setup was tested with two different aerosol sampling units during field campaigns in Berlin. In summer 2024, the Metrohm AeRosol Sampler (MARS) was operated with an extraction pH of 6.5 providing neutral reference extraction conditions. In winter 2025, a particle-into-liquid sampler (PILS) was applied using an extraction pH of 4.5 to probe iron solubility and speciation under mildly acidic, cloud-water-relevant extraction conditions. Limits of quantification (LOQ) for Fe(II) determination were 1.6 ng m⁻³ and 1.0 ng m⁻³ for the MARS-FIA and PILS-FIA setups, respectively, with ambient ws-Fe concentrations ranging from below LOQ to 47 ng m⁻³. Both setups yielded robust online measurements; however, the PILS-FIA working at pH 4.5 underestimated ws-Fe compared to filter sampling and extraction. This discrepancy can be attributed to the shorter extraction time in the PILS system, highlighting the influence of extraction duration on the measured iron concentration. Since soluble iron drives important tropospheric aqueous-phase reactions like hydroxyl radical formation through Fenton chemistry, the speciation data provided by the presented setup could improve model representations of atmospheric iron processes.

1 Introduction

Atmospheric soluble iron concentration is of great interest for atmospheric processes, public health and ocean biochemistry. In the global biogeochemical iron cycle, atmospheric iron supports marine productivity, particularly in open ocean regions where it is suggested to regulate and even limit phytoplankton growth (Browning and Moore, 2023; Moore et al., 2013). The bioavailable fraction of atmospheric iron is assumed to be soluble (Raiswell et al., 2008; Fan et al., 2006) and can influence the ocean-atmosphere carbon cycling which in turn affects Earth's climate (Hutchins and Tagliabue, 2024; Shao et al., 2011; Jickells et al., 2005).

Furthermore, airborne soluble iron is present in either Fe(II) or Fe(III) and can thus participate in multiple atmospheric processes altering the chemical composition of aerosols (Al-Abadleh, 2024; Pehkonen et al., 1993). For example, previous studies have shown that soluble iron impacts on the formation of secondary organic aerosol (Lüchtrath et al., 2024; Chu et al., 2017) and depending on the oxidation state, light conditions and presence of hydrogen peroxide (H_2O_2) can lead to the formation of light absorbing particles by reacting with phenolic precursors (Lüchtrath et al., 2025; De Haan et al., 2024; Hopstock et al., 2023; Slikboer et al., 2015) thus having a direct impact on the Earth's radiative budget.

In the aqueous phase, iron acts as a major catalyst for hydroxyl (OH) radical formation through Fenton ($\text{Fe(II)} + \text{H}_2\text{O}_2$) and photo-Fenton ($\text{Fe(III)} + \text{light} + \text{H}_2\text{O}_2$) reactions and thus enhancing the oxidation capacity of aerosol particles in atmospheric droplets (Tilgner and Herrmann, 2018; Herrmann et al., 2015; Arakaki and Faust, 1998; Zepp et al., 1992; Fenton, 1894).

On a global scale, mineral dust is the primary source of atmospheric iron; Ito and Shi, (2016) estimated that it contributes about 98 % of the total atmospheric iron budget. Freshly emitted dust exhibits very low iron solubility (Longo et al., 2016; Mahowald et al., 2009; Luo et al., 2005). During atmospheric transport, Fe-bearing minerals can dissolve through three main pathways, which are proton-promoted, ligand promoted and reductive dissolution (Al-Abadleh et al., 2024; Chen and Grassian, 2013; Rubasinghege et al., 2010). These three mechanisms are influenced by various factors like pH, particle size, presence of solar radiation, crystallinity of the Fe-bearing mineral and the Fe-organic complexes (Liu et al., 2022; Meskhidze et al., 2017; Paris and Desboeufs, 2013; Journet et al., 2008). Over the past decades, research consistently demonstrates that iron dissolution rates are highest under acidic conditions ($\text{pH} < 4$), particularly when exposed to solar radiation and oxalate (e.g. Chen and Grassian, 2013) with nanometer-sized, amorphous iron, especially from combustion sources (e.g. Baldo et al., 2022; Ito et al., 2019).

Under typical environmental conditions, Fe(II) starts to hydrolyse at $\text{pH} > 8$, whereas Fe(III) hydrolysis begins already at $\text{pH} > 3$ (Langmuir, 1997). Atmospheric aerosols, cloud and fog droplets exhibit acidity spanning approximately 5 pH units (Pye et al., 2020). Typical pH values for cloud droplets range from 3 to 6 (Pye et al., 2020). However, most cloud droplets do not precipitate as rain; instead, they evaporate, leaving a residual thin water film around dust particles. The wet aerosols can have aqueous-phase pH values below 2 (Pye et al., 2020). Shi et al. (2015) simulated the cycling of Fe-containing particles between wet aerosols ($\text{pH} 1\text{--}2$) and cloud droplets ($\text{pH} 5\text{--}6$). They found that acidic wet aerosol conditions promote rapid dissolution of low soluble Fe-containing particles, whereas at higher pH in cloud droplets precipitation of Fe-rich nanoparticles is favored, which can rapidly re-dissolve upon droplet evaporation. The authors further emphasized that the duration of the acidic aerosol stage increases the amount of soluble iron.

As illustrated in Figure 1, combustion processes like biomass burning, industrial production but also traffic contribute only few percent to the total amount of atmospheric iron (Ito and Shi, 2016; Luo et al., 2008), but possibly make up 40–100 % of the total soluble Fe fraction (Ito, 2015; Sholkovitz et al., 2009; Luo et al., 2008). The concentrations of dissolved iron in fog and cloud water can therefore vary locally depending on environmental conditions and iron emission source, ranging between 0.002 and $647 \mu\text{molL}^{-1}$ (Bianco et al., 2020; Deguillaume et al., 2005).

In atmospheric science literature, solubility is often defined as the percentage of dissolved Fe, measured in the filtrate after passing through a 0.2–0.45 μm pore size filter, relative to the total Fe content in the bulk aerosol sample (Shi et al., 2012). Because the concentration of Fe in the filtrate (and thus its measured solubility) depends on pH, we use the term “water-soluble (ws) Fe” in this study. This includes Fe measured both in neutral water (Seradest, pH 6.5) and under slightly acidic conditions (pH 4.5), which simulate cloud water environments.

A common method to determine water-soluble Fe(II) (ws-Fe(II)) in ambient aerosols (Kuang et al., 2020; Oakes et al., 2010; Rastogi et al., 2009) spectrophotometrically is the reaction between dissolved Fe(II) and ferrozine leading to the formation of a stable magenta-coloured complex developed by Stookey (1970). The reduction of dissolved Fe(III) to Fe(II) by a reductant like hydroxyl ammonium hydrochloride (HA) enables the determination of total ws-Fe and has been extensively used (Lei et al., 2023; Majestic et al., 2006; Stookey, 1970). The applied reduction time varies from some minutes (Lei et al., 2023; Kuang et al., 2020) to several hours (Yang et al., 2021).

The principle of flow injection analysis (FIA) firstly introduced by Nagy et al. (1970) is the precise introduction of sample volumes into a continuous, bubble-free stream, enabling automated analyses that are fast, accurate, and widely applicable. FIA setups have been used to determine ws-Fe(II) and total ws-Fe of different origins as natural water, waste water, potato leaves or human hair (e.g. Pullin and Cabaniss, 2001; Pascual-Reguera et al., 1997).

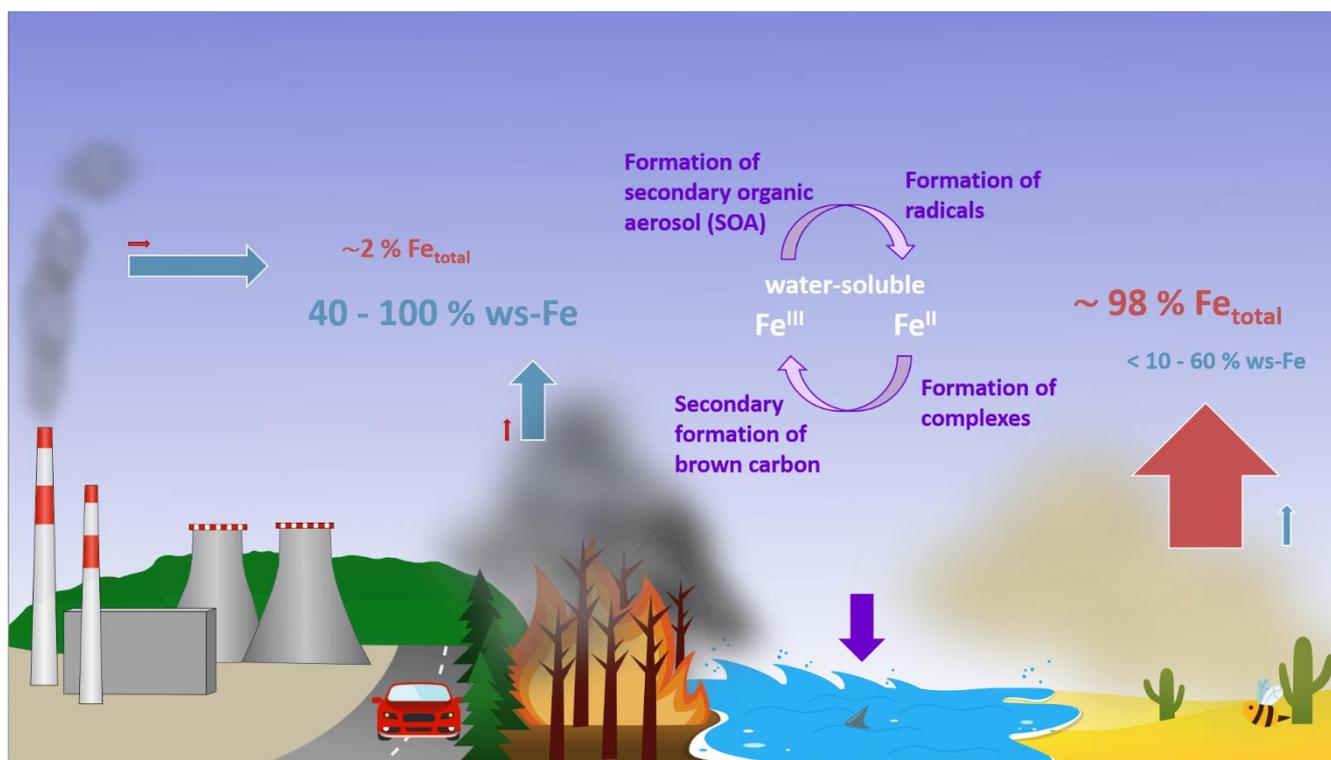


Figure 1: Sources, sinks and processes of atmospheric water-soluble iron

Aerosols are typically collected on filter for 12-24 h and analysed offline afterwards. The offline analysis limits the investigation of time resolved variability in concentrations and speciation of ws-Fe. Furthermore, the redox state of iron can change during collection and filter storage. Rastogi et al. (2009) developed the first online technique for determining water-soluble Fe(II) in ambient aerosols using a particle-into-liquid sampler coupled with a continuous flow ferrozine method. Building on the work of Rastogi et al. (2009), we present an online method combining FIA and particle-into-liquid sampling to quantify ws-Fe(II), total ws-Fe, and thereby ws-Fe(III), advancing insights into ws-Fe sources, processes of Fe dissolution and the role of iron chemistry in atmospheric processes (Figure 1).

2 Methods

2.1 Chemicals and Solution Preparation

Except for the glass volumetric flasks, only plastic bottles and beakers were used to avoid iron cross contamination. All vessels were cleaned by soaking in 0.03 M HNO₃ and rinsed with Seradest water (Seradest S750, Veolia Water Technologies, Germany). The 0.03 M HNO₃ was prepared from bidistilled water and HNO₃ (65 %, Suprapur, Merck, Germany). A 0.8 mM HNO₃ solution was prepared to achieve a pH of 3–3.5, while a 0.04 mM HNO₃ solution was used to obtain a pH of 4.5. All working standards and solvents for the FIA system were freshly prepared daily. The iron working standards (0.5-50 µg L⁻¹) were prepared by dilution of a 1 g L⁻¹ dissolved Fe(II) stock solution (acidified to pH1 by HCl) of FeSO₄·7H₂O (≥99% p.a., Carl Roth GmbH, Germany) and a 1 g L⁻¹ dissolved Fe(III) stock solution (acidified to pH1 by HCl) of (NH₄)₂Fe(SO₄)₂·6H₂O (≥ 98%, Carl Roth GmbH, Germany). Ferrozine solutions were prepared by dissolving 133 mg Ferrozine, 3-(2-pyridyl)-5,6-diphenyl-1,2,4-triazine-4',4'-disulfonic acid sodium salt (Iron reagent, hydrate, 95+%, pure, Thermo Scientific Chemicals, Germany) in 100 mL Seradest water, resulting in a 2.7 mM solution. As a reduction reagent, 19.3 mg hydroxylamine hydrochloride (99.9 %, Thermo Scientific Chemicals, Germany) was dissolved in 50 mL Seradest water. For cleaning the FIA system and the liquid waveguide capillary cell (LWCC), methanol, 2 M HCl and 2 % Hellmanex (Hellma Analytics GmbH & Co. KG, Germany) were used.

2.2 Definition of Water-Soluble Iron

The lack of a standardized protocol for determining trace metal solubility, including Fe, has been widely discussed in the literature (e.g. Tang et al., 2025; Perron et al., 2020; Meskhidze et al., 2016). Several studies have demonstrated that leaching or extraction procedures, including different chemical composition and pH value of the solutions as well as different contact time, strongly influence the measured metal's solubility (e.g. Li et al., 2023; Tang et al., 2025; Perron et al., 2020; Meskhidze et al., 2016). Most comparative studies investigating the effect of leaching solutions on iron solubility have used ultrapure

water or organic buffers such as formate or acetate with a pH around 4.3 (e.g. Li et al., 2023; Perron et al., 2020; Majestic et al., 2006).


115 As no standard protocol exists, a variety of operational terms have been used in the literature to describe experimentally mobilised aerosol trace element fractions, including ‘soluble’, ‘labile’, ‘leachable’, ‘dissolved’, ‘readily accessible’, ‘bioaccessible’ and ‘bioavailable’, as summarized by Tang et al. (2025). The use of different extraction or leaching approaches and definitions complicate direct comparison of reported iron solubility and soluble iron concentrations across studies.

This study focuses on the analysis of the iron fraction which is soluble in Seradest water (pH6.5), used as a near-neutral reference condition, and Seradest water adjusted to pH 4.5 with HNO₃, providing mildly acidic, low-ionic-strength aqueous conditions representative of cloud-water acidity while minimizing additional chemistry introduced by adding buffering agents. The pH of the aqueous phase can vary widely, ranging from highly acidic conditions (pH<0) in deliquesced aerosols to neutral pH in rain and fog water (e.g. Pye et al., 2020; Herrmann et al., 2015). As discussed above, the solubility of atmospheric iron depends on particle size, chemical composition, photochemical activity and atmospheric processing, as well as on pH. To allow a clearer interpretation of our data, we therefore use the term *water-soluble iron* throughout this study, emphasizing that the reported values represent the fraction of iron that is soluble under neutral and mildly acidic aqueous conditions relevant to cloud, fog and rain water.

A key advantage of the online approach is the high temporal resolution of the measurements; however, the method requires short extraction and reaction times for both ferrozine and the reducing reagent hydroxylamine (HA), as will be discussed in section 3.1.1. Consequently, the quantity reported as ws-Fe(II) is operationally defined by the reaction time of dissolved Fe(II) with ferrozine. The term total ws-Fe refers to the amount of Fe detected as dissolved Fe(II) after addition of HA, which reduces dissolved Fe(III) to Fe(II) prior to complexation with ferrozine.

2.3 Online Analysis System

135 A measurement setup consisting of a commercially available particle-into-liquid sampling unit and a custom-built flow injection analysis (FIA) system with a liquid waveguide capillary cell (LWCC) was developed to detect, in online mode, the concentration and oxidation state of water-soluble atmospheric soluble iron. Two commercially available sampling units were used: the Metrohm AeRosol Sampler (MARS; Metrohm Process Analytics, Filderstadt, Germany) and the Particle-Into-Liquid Sampler PILS BMI 4002 (Brechtel Manufacturing Inc., USA). Concentrations of ws-Fe(II) and total ws-Fe were quantified spectrophotometrically by the ferrozine method. Ferrozine and dissolved Fe(II) form a complex with a characteristic absorbance maximum at $\lambda = 562$ nm (Stookey, 1970). Total ws-Fe was determined after reduction of dissolved Fe(III) to Fe(II) using hydroxylamine hydrochloride (HA) as reduction reagent. A scheme of the setup is shown in Figure 2. All dimensions and flow parameters are listed in Table 1. The system components will be explained in more detail in the following sections.

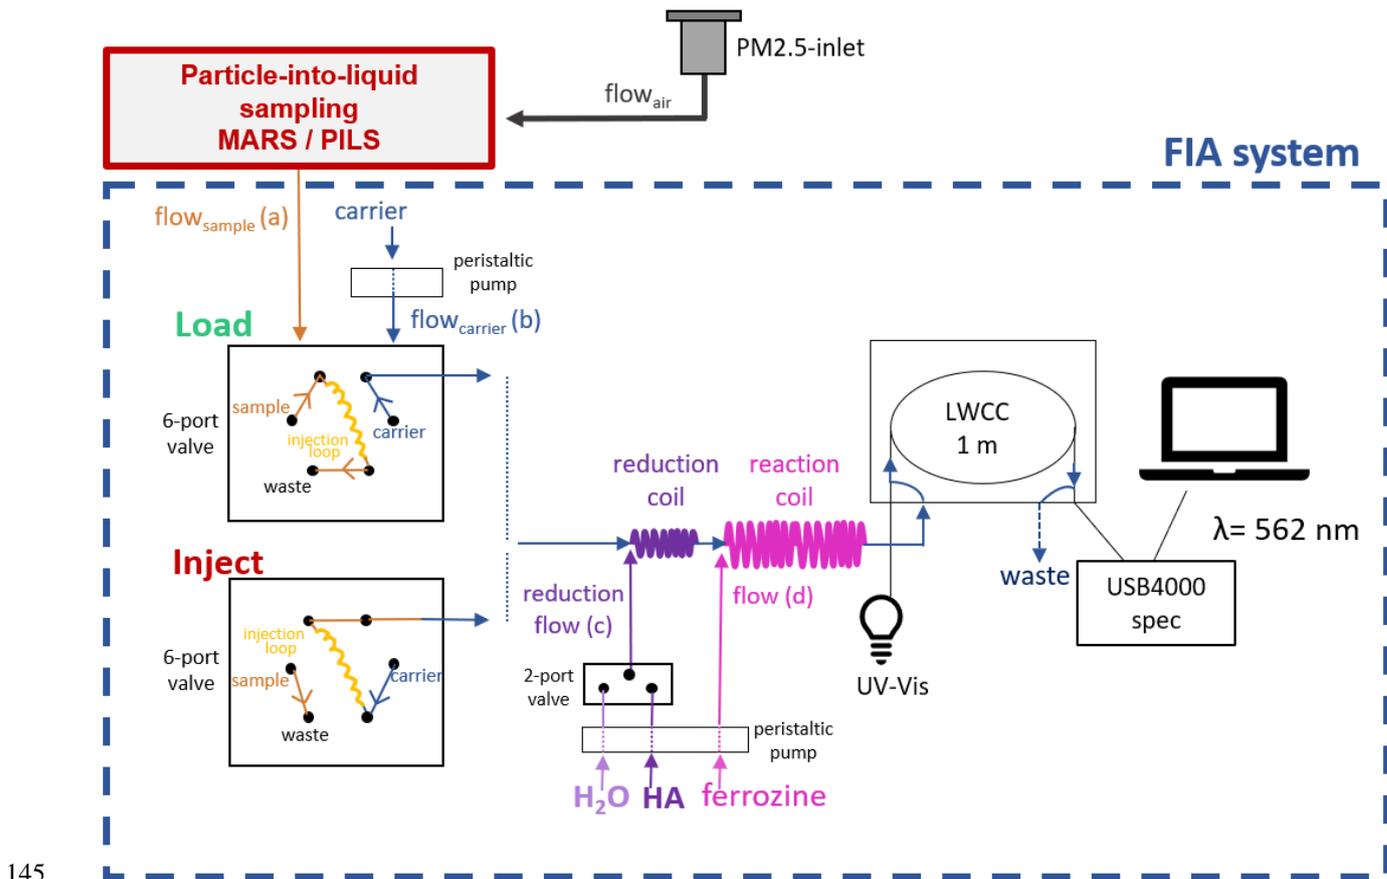

150

Figure 2: Schematic diagram of the measurement setup in detail. During LOAD mode, the aerosol sample solution is transferred into the injection loop of the six-port valve, while the carrier stream flows through the FIA system. After the injection loop is filled (10 min for the MARS-FIA and 12 min for the PILS-FIA), the automated six-port valve switches to INJECT mode. In INJECT mode, the carrier stream is directed through the injection loop, thereby pushing the sample toward the FIA. The sample is first transferred to a T-piece connected to a 2-port valve, where HA or H₂O are added alternately to the sample stream before entering the reduction coil. After passing the reduction coil, the sample stream enters a second T-piece where ferrozine is added prior to the reaction coil. Following the reaction coil, the sample enters the LWCC coupled to a spectrophotometer, where absorbance is measured.

155

2.3.1 Particle-into-liquid sampling units

160 Particle-into liquid sampling units are designed to enable an online analysis of ambient aerosol bulk composition. The basic
principle is based on particle growth into droplets through supersaturation of water vapor which are then collected in liquid
solution (e.g. Stieger et al., 2018; Weber et al., 2001). The Metrohm AeRosol Sampler (MARS) is part of the commercial
Monitor for AeRosols and Gases in ambient Air (MARGA, Metrohm, Applikon, Netherlands). Both, MARGA and PILS
165 measurements were conducted in several studies (e.g. Zeng et al., 2021; Stieger et al., 2019) and are thus validated approaches
for the online determination of water-soluble aerosol compounds.

Metrohm AeRosol Sampler (MARS)

The MARS sampler was connected to a PM_{2.5} inlet. The airflow of 1 m³ h⁻¹ is regulated by the usage of a critical orifice. The
air flow passes the Wet Rotator Denuder (WRD) which removes soluble gases from the air stream. Aerosols will not be
170 absorbed but follow the air stream due to their inertia. After having passed the WRD the air stream enters the Steam Jet Aerosol
Collector (SJAC) where supersaturated steam is introduced by a steamer. In the steamer chamber, the particles grow by
deliquescence. Due to their inertia the grown particles are separated by the cyclone and collected into the 1.2 mL sampling
volume on the bottom of the SJAC. The liquid sampled is continuously transferred through a 0.45µm syringe filter to the
injection loop of the FIA system. The sample flow to the FIA system was adjusted to 0.1 mLmin⁻¹. The sample concentration
175 factor (SCF) describes the ratio between the concentration in the atmosphere (c_{air}) and the liquid sample (c_{sample}) (Eq.1). The
MARS-FIA system had an SCF of 6. As no internal standard was used no dilution factor was applied.

$$c_{air} [ng\ m^{-3}] = c_{sample} [\mu g\ L^{-1}] \cdot SCF \quad \text{Eq.1}$$

Particle Into Liquid Sampler (PILS)

The PILS BMI4002 is a modification of the PILS instrument described by Weber et al. (2001). Its setup and operation mode
180 were described in detailed by Sorooshian et al. (2006). The PILS was used in online mode and operated at an air flow rate of
14.6 Lmin⁻¹ with a 2.5 µm diameter-cut cyclone at the inlet. No denuders were installed. In the condensation chamber, the
ambient air mixes with steam leading to supersaturation and therefore particle activation. The activated particles grow to >1 µm
diameter before they reach the impaction plate (Sorooshian et al., 2006). A wash flow of 0.065 mL min⁻¹ transports the
impacted droplets down the impactor plate from where they are transferred to the FIA system at a sample flow rate
185 (Flow_{Sample} (a)) of 0.05 mL min⁻¹. The pH of an average droplet can be expected to be 5.6 (Ma, 2004; Sorooshian et al., 2006).
To test whether Fe-solubility is increased by lowering the pH of the sample, the wash flow was slightly acidified to pH 4.5
using 0.04 mM HNO₃. During particle collection, liquid from the droplets and the transport flow solution can dilute the sample.
Additionally, water condenses on the impaction plate. Orsini et al. (2003) quantified this additional water as 5 to 20 µL min⁻¹.
As no internal standard was used in this study and the wash flow was 1.3 times higher than the sample flow, a dilution factor

190 of 1.5 was applied, assuming an average additional condensed water contribution of $10 \mu\text{L min}^{-1}$. The SCF for the PILS system was 5.13.

Blank measurements of both sampling units were conducted regularly by directing the airflow through a HEPA zero filter (HEPA-CAP, Whatman, UK). The filter was connected for one hour prior to measurement. Blank values were then determined from the subsequent two hours of sampling. The limit of quantification (LOQ) was defined as ten times and the limit of detection (LOD) three times the standard deviation of the blank values (Eq.2 & 3) and were determined for ws-Fe(II) and total ws-Fe.

$$LOD = 3 \cdot \sigma_{blanks} \quad \text{Eq. 2}$$

$$LOQ = 10 \cdot \sigma_{blanks} \quad \text{Eq. 3}$$

Table 1: Overview of dimensions and operational parameters for MARS - and PILS-FIA systems

	MARS	PILS
Cut off diameter	2.5 μm	2.5 μm
Flow _{air}	16.7 L min ⁻¹	14.6 L min ⁻¹
SCF	6	5.13
Injection volume	600 μL	400 μL
Flow _{sample} (a)	0.1 mL min ⁻¹	0.05 mL min ⁻¹
Sampling time	8 min	10 min
Injection intervall	10 min	12 min
pH of sampling flow	5.5 – 6.0	4.5
FIA flow _{carrier} (b)	1.0 mL min ⁻¹	0.5 mL min ⁻¹
FIA ferrozine flow (c)	0.1 mL min ⁻¹	0.05 mL min ⁻¹
FIA reduction flow (d)	0.1 mL min ⁻¹	0.05 mL min ⁻¹
Reaction coil	800 cm	800 cm
Reaction time	78 s	157 s
Reduction coil	200 cm	200 cm
Reduction time	20 s	40 s
Total tubing length	1080 cm	1080 cm
Tubing diameter	0.5 mm	0.5 mm
LWCC volume	250 μL	250 μL
LOD _{Fe, total}	0.48 n gm ⁻³	0.15 ng m ⁻³
LOD _{Fe(II)}	0.39 n gm ⁻³	0.3 ng m ⁻³
LOQ _{Fe, total}	1.6 n gm ⁻³	0.5 ng m ⁻³
LOQ _{Fe(II)}	1.3 n gm ⁻³	1.0 ng m ⁻³
Blank _{Fe total}	1.84± 0.16 n gm ⁻³	3.51±0.10 n gm ⁻³
Blank _{Fe2+}	1.01± 0.12 n gm ⁻³	0.84± 0.05 ng m ⁻³

200 2.3.2 Flow Injection Analysis Unit

A three-line flow injection analysis system was developed to quantify soluble iron in liquid samples using spectrophotometric detection. Ferrous iron (Fe(II)) forms a stable magenta complex with ferrozine which absorbs at 562 nm, enabling its detection. This method was originally introduced by Stookey (1970). A previous reduction of present dissolved Fe(III) further enables the determination of the total soluble iron fraction.

$$total\ ws-Fe = ws-Fe(II) + ws-Fe(III) \quad \text{Eq. 4}$$

205

This FIA system includes two peristaltic pumps (ISMATEC, IPS 8), a common six-port valve used in HPLC systems (BESTA, Germany) with an injection loop, a two-way switching pinch valve (ASCO S306.02-Z530A), a 2 m reduction coil with an inner diameter of 0.5 mm and a volume of 0.4 mL, an 8 m reaction coil with an inner diameter of 0.5 mm and a volume of 1.6 mL, a UV-Vis light-source (DH-2000-BAL, Ocean Optics, Germany), a USB-Spectrophotometer (USB4000-XR1-ES, 210 Ocean Optics, Germany) and a liquid waveguide capillary cell (LWCC 3100, World Precision Instruments, Friedberg, Germany, 100 cm pathlength, 250 μ L internal volume, 0.5 mm inner diameter) (see Figure 2). The valve circuit of the six-port valve and the two-way pinch valve were controlled with a microcontroller (Arduino Nano). Software for data acquisition was written in LabView 2017 based on Ocean Optics USB4000 code.

During LOAD mode of the six-port valve, a continuous sample flow from the MARS or PILS system was collected into the 215 injection loop (600 μ L for MARS and 400 μ L for PILS), both exceeding at least 1.5 times the volume of the LWCC (see Figure 2). Due to the different sample flow rates (MARS: 0.1 mL min⁻¹; PILS: 0.05 mL min⁻¹), a smaller injection loop volume was used for the PILS-FIA system compared to the MARS-FIA system to achieve comparable injection time resolution. While the sample solution filled the injection loop, the carrier stream passed through the FIA system, providing the baseline signal. The carrier flow rate was set to 1.0 mL min⁻¹ for the MARS-FIA system and 0.5 mL min⁻¹ for the PILS-FIA system. The pH 220 of the carrier stream was adjusted to match the pH of the respective sample flow (pH 6.5 for MARS and pH 4.5 for PILS).

To ensure complete filling of the injection loop, sampling times of 8 min for the MARS-FIA system and 10 min for the PILS-FIA system were applied. Accordingly, the six-port valve switched from LOAD to INJECT mode after 8 min (MARS-FIA) and 10 min (PILS-FIA). During INJECT mode, the sample solution was injected into the carrier stream (see Figure 2). At the first mixing point, either hydroxylamine hydrochloride (HA) solution or Seradest water (H₂O) was introduced into the carrier 225 stream via a two-port switching valve (flow ratio carrier : HA/H₂O = 10 : 1). The injection valve was switched back to LOAD mode after 2 min, so that fresh extractant solution was filled into the loop thereby decreasing waiting time for the subsequent injection and increasing the sampling frequency.

For each LOAD-INJECT cycle, only one reagent was added to the sample stream. The addition of HA and H₂O was alternated between consecutive LOAD cycles, such that HA was added during one cycle and H₂O during the subsequent cycle. The two- 230 port valve was switched during each LOAD mode after the peak of the previous sample had been fully detected. Because the

addition of HA caused a baseline shift, the switching between HA and H₂O was carefully timed to occur between two consecutive peaks.

After passing the first mixing sample stream entered the reduction coil, where dissolved Fe(III) was reduced to Fe(II) only in the presence of HA. At the second mixing point, ferrozine was introduced into the sample stream (flow ratio ferrozine:carrier 1:10) before it entered the reaction coil. In previous online systems for ws-Fe(II) detection, ferrozine concentrations around 5 mM were commonly used (e.g. Rastogi et al., 2009; Majestic et al., 2006), typically added to the sample at a 1:10 ratio. In this study, a lower ferrozine concentration of 2.7 mM was sufficient for complete complexation of dissolved Fe(II), while also reducing chemical consumption. Experiments with dissolved Fe(II)-standard solutions indicated that 95 % of the maximum absorbance of the magenta- coloured Fe(II)-ferrozine complex was already reached after 70 seconds, allowing short reaction times (~80 s for MARS-FIA and ~160 s for PILS-FIA). Due to the short reaction time, reduction of dissolved Fe(III) by ferrozine alone was not observed as has been reported in previous studies (Murray and Gill, 1978). As the pH of the sample flow is not expected to be below pH 4.5, which is in the working range of ferrozine as a complexing agent (Zhang et al., 2001; Stookey, 1970), no buffer was used. After passing the reaction coil, the sample enters the LWCC. To prevent the formation of air bubbles due to outgassing, a PTFE capillary (0.5 mm inner diameter, 350 mm length; Metrohm AG, Germany) was attached to the outlet of the LWCC, as it increases the backpressure within the LWCC. The sample absorbance was determined at $\lambda = 562$ nm relative to $\lambda = 700$ nm. The average baseline was determined over a 75-second interval, from 2 minutes to 45 seconds before the peak, and subtracted from the signal. Quantification using peak height gave better precision than using peak area and was therefore applied in this study. All values were subsequently corrected for blank measurements.

2.3.3 Calibration and Daily Maintenance

The FIA system was regularly calibrated with 3–5 dissolved Fe(II) standards ranging from 0.5 to 40 $\mu\text{g L}^{-1}$, freshly diluted from a 1 g L^{-1} acidified stock solution. Daily calibration was performed with a 5 $\mu\text{g L}^{-1}$ Fe(II) standard. While Fe(II) is typically stabilized in 0.01 M HCl (Zhang et al., 2001) due to slower oxidation rate in acidic conditions (Millero et al., 1987), neutral pH standards were used here to match sample conditions and yielded reproducible results. For each measurement sequence, a single dissolved Fe(III) standards of pH 3.5 were regularly used to assess reduction efficiency. The standards showed improved stability and reproducibility when acidified to pH 3.5 compared to neutral pH conditions as dissolved Fe(III) hydrolysis occurs at $\text{pH} > 3$ while dissolved Fe(II) hydrolysis occurs at $\text{pH} > 8$ (Langmuir, 1997). An optimum pH range of 4–9 for the Fe(II)-ferrozine-complex formation was stated by Stookey (1970), but calibrating with dissolved Fe(II) standards of pH 3.5 gave the same results compared to calibrating with neutral pH, underlining that the ferrozine method also works at pH 3.5. To prevent the accumulation of the Fe-ferrozine complex onto the LWCC wall, the LWCC was daily cleaned with 2 % Hellmanex, methanol and 2 M HCl. FIA tubing was washed with 2 M HCl regularly to prevent the precipitation of iron oxides within the tubing.

2.4 Test Experiments and Instrument Evaluation

2.4.1 Test Experiments

265 Following the development of the FIA system, the setup was connected to MARS and tested during a two-week measurement
campaign in June 2024 in Berlin, Germany. The system was deployed inside a measurement container located at the main
campus of Technische Universität (TU) Berlin, close to the six-lane road “Straße des 17. Juni.” During the campaign, particle
size distributions were measured using an ELPI+ (Dekati, Finland), and equivalent black carbon (BC) concentrations were
determined with an aethalometer (MA200, AethLabs, USA). After this initial test campaign, the setup was optimized by
270 adjusting the pH of the extraction medium. A second one-week campaign was conducted in March 2025 on the terrace of an
institute building at the TU Berlin campus. This time, a PILS was used as the sampling unit, with an acidified sample flow at
pH 4.5. BC concentrations were again measured using the aethalometer MA200. PM_{2.5} concentrations were obtained from the
background monitoring stations in districts of Berlin (i.e. Wedding, Neukölln, and Mitte), which are part of the Berlin Air
Quality Monitoring Network (BLUME).

275

2.4.2 Offline Measurement

To evaluate the results from the online instruments, filter samples were collected during the test field campaigns in Berlin.
Additional filter samples were taken at a contrasting location to assess potential application environments: Mace Head, Ireland
(autumn 2024), representing background North Atlantic marine air (O'Connor et al., 2008). As different filter samplers, air
280 volumes, filter types and diameter were used at the different locations, all parameters are listed in Table 2. The filters from
Mace Head were stored frozen and transported to Berlin frozen. The filters in Berlin were stored at room temperature and in
the dark before extraction.

Iron solubility is strongly influenced by pH – lower pH values lead to increased solubility (Liu and Millero, 2002, 1999). Based
on the mean pH values reported by Pye et al. (2020) for 93 studies at 48 European locations between 1988 and 2018, the
285 average pH of cloud water in Europe is approximately 4.5. This value lies within the optimal pH range of the ferrozine method
and was therefore selected for comparison with neutral pH (pH 6.5) conditions.

To assess the effect of pH reduction on ws- Fe(II) concentration, filter cuts were extracted in Seradest water at pH 4.5 and at
pH 6.5 for 1 h in a horizontal shaker. Different cut sizes were used depending on the used particle collector (see Table 2). The
extracts were filtered through a 0.45 µm polyamide syringe filter (Chromatographie Handel Mueller, Germany) before they
290 were injected into the FIA-system for ws-Fe(II) and total ws-Fe determination. Samples were directly analysed after extraction
to minimize hydrolysis and precipitation of dissolved Fe(III) as well as oxidation of Fe(II) to Fe(III).

Extraction time and extraction pH vary across different studies published; for example, Chen and Siefert (2003) report that a maximum concentration of labile Fe was reached after 90 min at pH 4.5. To evaluate extraction efficiency at pH 4.5 for the much shorter extraction times typical of particle-into-liquid sampling units (only a few minutes), filters from the second campaign were extracted for 1, 5, 10 and 30 min. The total ws-Fe(II) concentration was determined directly after extraction using the FIA system, and extraction efficiency was then calculated.

Table 2: Summary of filter sampling parameters at the different locations

Station	Sampling duration	Sampler	Cut-off Diameter	Sampling Volume	Filter	Dimension of Filter Cut [mm]	Extraction volume [mL]
Berlin, Straße des 17. Juni	24 h sampling	Lekel, SEQ 47/50	PM 2.5	2.3 m ³ h ⁻¹	47 mm, Munktell MK360	Ø 15	3
Berlin, Campus TU Berlin	24 h sampling	Digitel	PM 2.5	30 m ³ h ⁻¹	150 mm, QM-A, Whatman	Ø 25	5
Mace Head, Ireland	5-10 d sampling	HiVol sampler	PM 1.5	97.2 m ³ h ⁻¹	slotted filters, Whatman41	30 x 10	5

300 3 Results and Discussion

3.1. Characteristics of the FIA system

3.1.1 Calibration and Limit of Quantification

Based on measurements of calibration standards and system blanks, the linear working range, the sensitivity, the limit of detection (LOD) and the limit of quantification (LOQ) of the FIA system were obtained.

305 A universal calibration curve from 0.5 to 40 µg L⁻¹ dissolved Fe(II) was determined as an average linear regression of ten individual calibration measurements taken over the course of one year (Table A1), based on measurements performed on different days in the laboratory and under varying conditions in the field, including minor fluctuations in flow rates and changes in pump tubing. The individual linear regression slope values ranged from 0.0206 to 0.0280 (1/µg L⁻¹), with an average of 0.0242 ± 0.0024 (1/µg L⁻¹). The intercept was -0.0023 ± 0.0076 and R² was 0.996. The low standard deviation of the slopes
 310 (<10 %) demonstrates good reproducibility for calibration slopes, highlighting the robustness of the system under varying operational conditions, and confirming its suitability for field deployment. Reduction efficiency was tested with single dissolved Fe(III) standards of pH 3.5 and showed high efficiency, varying between 80-117% relative to dissolved Fe(II) when standards were freshly prepared. A decrease in reduction efficiency was observed with increasing age of the dissolved Fe(III) standards likely due to the formation of hydrolysed Fe(III) species which are not rapidly reduced by HA. This observation
 315 highlights that, under the short reduction times in the FIA system, less reactive or less reducible Fe(III) species may not be fully reduced. Previous studies have used HA as reducing solution in flow injection systems applying very short reaction times (HA and ferrozine together) of approximately 1 minute (e.g. Pullin and Cabaniss, 2001; Teixeira and Rocha, 2007). In the

presented systems the reduction times were 20 s for the MARS and 40 s for the PILS system. The reaction times with ferrozine were 78 s for the MARS and 157 s for the PILS system (Table 1). Therefore, the total time for the reduction of dissolved Fe(III) to Fe(II) was 98 s for the MARS and 197 s for the PILS system. Pullin et al. (2007), using an acetate buffer carrier of pH 4.0 and a reaction temperature of 65°C, reported 100 % reduction efficiency by adding acetic acid to the carrier and colour reagent suggesting that the acetate buffer forms a complex with the dissolved Fe(III). As no buffer solution was used in the present FIA apparatus, the addition of acetic acid had no effect on reduction efficiency when injecting aged Fe(III) standards. Heating of the reduction coil in a water-bath as reported by Pullin et al. (2007) was not applied to reduce the technical complexity for a system which is intended to run continuously for a long period of time. Similarly, heating was not applied in many other FIA systems designed for ws-Fe(II)/(III) determination (e.g. Attiyat et al., 2011; Teixeira and Rocha, 2007). Luther et al. (1996) reported incomplete reduction of dissolved Fe(III) by HA in the presence of humic-like substances. To acknowledge this limitation imposed by the operational given reduction time, further on we use the term reducible Fe(III) instead of ws-Fe(III). This also underlines that total-ws Fe is defined by the kinetics of the FIA system and might also underestimate the total ws-Fe concentration compared to studies with longer reduction times.

The average blank concentrations from the test field campaigns (n=2) are listed in Table 1. Generally, the mean blank concentrations of total ws-Fe (MARS-FIA: 1.84 ng m⁻³, PILS-FIA: 3.51 ng m⁻³) are higher compared to the mean blank concentrations of ws-Fe(II) (MARS-FIA: 1.01 ng m⁻³, PILS-FIA: 0.84 ng m⁻³). The PILS-FIA-system shows higher blank values for total soluble iron than the MARS-FIA system. An advantage of the MARS is the fast and simple washing procedure, as the SJAC can quickly be dismantled and cleaned in isopropanol in an ultrasonic bath.

The lowest LOD with 0.15 ng m⁻³ was determined for total ws-Fe using the PILS-FIA setup (Table 1). The highest LOD with 0.48 ng m⁻³ (Table 1) was determined for total ws-Fe using the MARS-FIA setup. The LOQ from the blank measurement of total ws-Fe was 1.6 ng m⁻³ for the MARS-FIA and 1.0 ng m⁻³ for the PILS-FIA (Table 1). The blank uncorrected LOQ for the MARS-FIA system was 2.7 ng m⁻³, which corresponds to 0.45 µg L⁻¹, and 5.1 ng m⁻³ for the PILS-FIA system, which corresponds to 1.15 µg L⁻¹. These liquid concentrations are at the lower end of the calibration range.

3.1.2 Effect of pH and Extraction Time


As iron solubility is directly influenced by pH, which typically ranges between 3 and 6 in cloud water (Pye et al., 2020), filters were extracted at near-neutral reference pH (6.5) and cloud water related pH (4.5) (see section 2.4.2).

At pH 6.5, the lowest ws-Fe concentrations were found at Mace Head, Ireland (Table 3, Filters C1–C5), with ws-Fe(II) ranging from <LOQ to 0.04 ng m⁻³. Total ws-Fe concentrations were only slightly higher (LOQ–0.06 ng m⁻³), resulting in ws-Fe(II)/total ws-Fe ratios around 0.8. These high ratios indicate that nearly all water-soluble Fe was present as dissolved Fe(II). When extracted at pH 4.5, both ws-Fe(II) and total ws-Fe concentrations increased, reaching 0.07–0.16 ng m⁻³ and 0.13–.29 ng m⁻³, respectively. The relative increase was higher for total ws-Fe than for ws-Fe(II), leading to a lower ws-Fe(II)/total ws-Fe ratio of 0.45–0.70. This indicates that under slightly acidic conditions, more reducible Fe(III)

350 compounds dissolved than Fe(II), as expected from the enhanced solubility of Fe(III) oxides and Fe(III) hydroxides at lower pH (e.g. Balsamo Crespo et al., 2023; Langmuir, 1997; Pye et al., 2020). The very low ws-Fe(II) and total ws-Fe concentrations evidence the clean air and pristine marine conditions at Mace Head.

In contrast to the clean marine air masses sampled at Mace Head, Berlin urban air is strongly influenced by anthropogenic activity, which is reflected in higher concentrations of both ws-Fe(II) and total ws-Fe (Table 3). During the second test
355 campaign in winter 2025 (Filters B5–B9), extraction at pH 6.5 yielded ws-Fe(II) concentrations between 1.1 and 7.5 ng m⁻³ and total ws-Fe between 3.2 and 16.47 ng m⁻³. The resulting ws-Fe(II)/total ws-Fe ratios of 0.22–0.46 indicate that a large fraction of water-soluble iron was present as reducible Fe(III) rather than ws-Fe(II). When filters were extracted for 1 h at pH 4.5, concentrations increased substantially: ws-Fe(II) increased to 10.78–21.63 ng m⁻³ and total ws-Fe to 11.76 – 5.47 ng m⁻³, resulting in an higher ws-Fe(II)/total ws-Fe ratios of 0.68 –0 .92. This result indicates that under mildly
360 acidic, cloud-water relevant conditions a large fraction of the dissolved iron is present as Fe(II). This enrichment may reflect the mobilisation of Fe that has previously undergone ligand-mediated dissolution and redox processing in the atmosphere, where organic ligands such as oxalate are known to increase iron dissolution by complexation and facilitate photoreduction of Fe(III) to Fe(II) under mildly acidic conditions (Shi et al., 2012). In addition, complexation with organic ligands has been shown to stabilize dissolved Fe(II) in rain water of pH 4.5 (Kieber et al., 2005). Overall, this demonstrates that the extraction
365 pH can affect both the amount and speciation of the water-soluble iron.

The speciation between ws-Fe(II) and ws-Fe(III) in ambient atmospheric particles has been investigated in several studies before (e.g. Gao et al., 2019, 2020; Kuang et al., 2017; Majestic et al., 2006). This speciation is useful for identifying sources of water-soluble iron in dust because the ws-Fe(II)/ws-Fe(III) ratio varies according to origin. For instance, previous studies have revealed that diesel exhaust particles typically exhibit low water-soluble Fe(II)/Fe(III) ratios (Valavanidis et al., 2000),
370 whereas particles originating from biomass burning exhibit notably higher ratios (Wang et al., 2022; Fu et al., 2012). Our extracted filters further show that iron solubility and speciation are strongly influenced by pH. The observation aligns with findings of Majestic et al. (2006), observing that ws-Fe(II) to reducible Fe(III) ratios vary between extractions performed with Milli-Q water (pH 6.3) and those with acetate buffer (pH 4.3). This suggests that iron sources could be identified by determining the dissolved Fe species under different conditions. Therefore, it is important to consider pH dependence when
375 comparing water-soluble Fe(II)/Fe(III) speciation data from different studies.

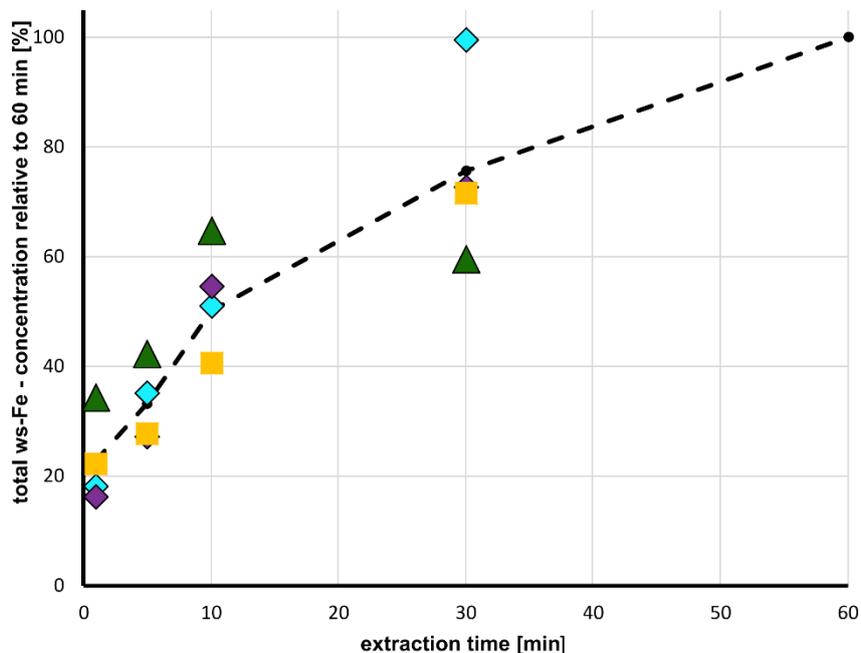

380 **Figure 3: Total ws-Fe concentration relative to the total ws-Fe (II) concentration after 60 min as a function of extraction time** for four filters (B5-B8) from the second field campaign. The filters were extracted in pH 4.5 solution and total ws-Fe was determined. Coloured symbols represent the efficiencies determined for the four different filter samples (B5-B8); the black dashed line indicates the average.

The extraction times within the MARS-FIA and PILS-FIA systems were shorter than in the 1 h offline filter extraction procedure. Particles not dissolved during sampling can remain suspended in the liquid stream if filtration is not applied. In the MARS-FIA setup, the liquid sample passed through a 0.45 μm syringe filter before entering the FIA system, whereas no filter was used in the PILS-FIA setup. In both setups, the transfer time from the sampling unit to the FIA system was approximately 2 min. The sampling time into the injection loop was 8 min for the MARS-FIA and 10 min for the PILS-FIA (Table 1) guaranteeing a complete filling of the injection loop with sample. After injection, the total residence time of the sample in the FIA system was 1 min 45 s for MARS-FIA and 3 min 30 s for PILS-FIA. Therefore, the total time that particles were in contact with the liquid phase was about 12 min in MARS-FIA and 16 min in PILS-FIA. To investigate the efficiency of extraction as a function of extraction time, filters from the second test campaign (filters B5-B8) representing cloud-water conditions were also analysed after 1, 5, 10 and 30 min of extraction at pH 4.5. The results are listed in Table A2, and the extraction efficiency, normalized to the concentration obtained after 1 h of extraction, is shown as a function of time in Figure 3. The coloured symbols represent the efficiencies determined for the four different filter samples, while the black dashed line indicates their average. After 1 min of extraction, only 20–30 % of the total ws-Fe was dissolved. After 10 min, the extracted fraction increased to 40–60 %. After 30 min, filter B7 (turquoise squares) already reached complete extraction relative to the 1 h filter extraction, whereas the efficiencies for the other three filters remained between 60 and 70 % (Figure 3).

385
390
395

Overall, these results show, that the extraction time is an important factor when determining the concentration of water-soluble iron at cloud-water relevant pH. As the extraction time in the online instruments is shorter compared to filter analysis, the concentration determined online might not represent the total extractable water-soluble iron fraction. Therefore, extraction time is an important factor to consider when comparing measurements and interpretations between different studies.

400

3.2. Test campaigns and First Field Application

Concentrations of ws-Fe(II) and total ws-Fe were measured with the online system and with offline filter samples during two test campaigns in Berlin, at *Straße des 17. Juni* in June 2024 and on the main campus of TU Berlin in March 2025.

3.2.1 Comparison of Online and Offline Measurements

405 The concentrations of ws- Fe(II) (light-red) and total ws- Fe (dark-red) measured online during the two test campaigns are shown in Figure 4. Shaded areas indicate values obtained from offline filter analysis. During the first campaign at *Straße des 17. Juni* in June 2024, online ws-Fe(II) and total ws-Fe concentrations varied between 1 and 9 ng m⁻³, except between 08.06.2024 and 09.06.2024, when total ws-Fe reached 50 ngm⁻³ (Figure 4a). On average, during the period the total online ws-Fe concentration was 5.2 ngm⁻³. Elevated water-soluble iron concentrations during this period of the first campaign were also
410 observed in the offline filter samples, with an average offline ws-Fe(II) concentration of 17.0 ngm⁻³ on 08.06.2024 (Table 3, Filter A4). Averaged online ws-Fe(II) concentrations from the MARS-FIA system for the corresponding period were 19.5 ngm⁻³.

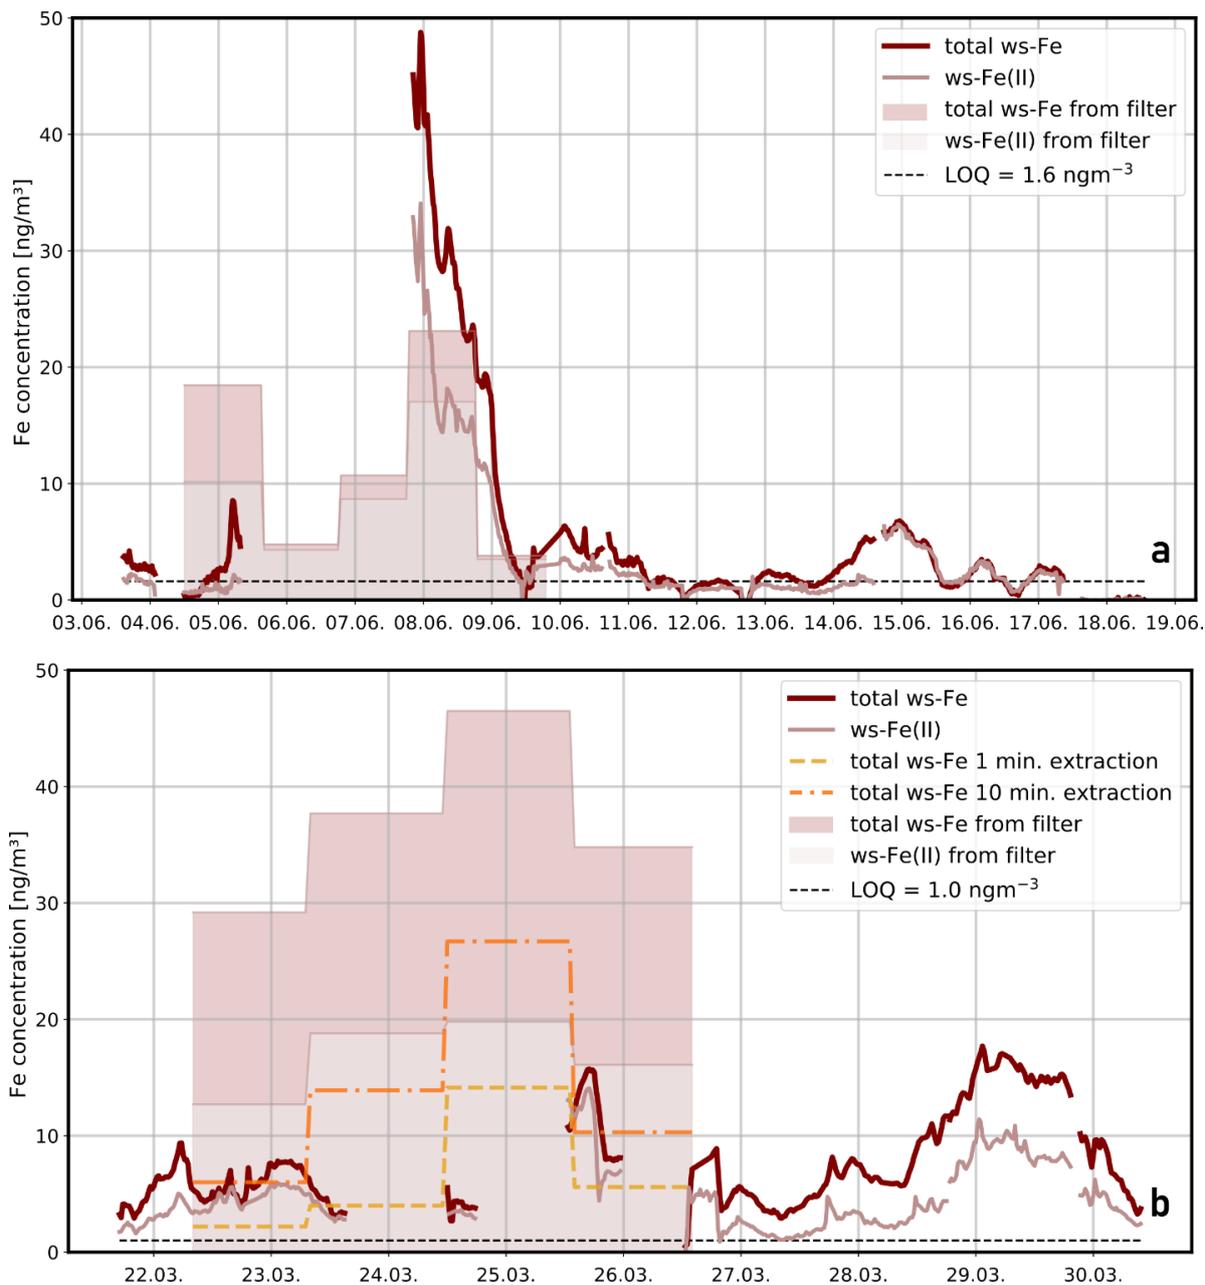


Figure 4: Temporal variability of total ws-Fe (red) and ws-Fe(II) (light-red) concentrations in particulate matter (PM_{2.5}) in Berlin:

415 a) First test campaign with MARS-FIA setup at the road *Straße des 17. Juni* from 03.06.-19.06.2024. The shaded areas represent the
 concentrations obtained by filter analysis with filter extraction in Seradest water. The black dashed line represents the LOQ from blank
 measurements. b) Second test campaign with PILS-FIA setup at TU Berlin Campus from 22.03.-30.03.2025. The shaded areas represent the
 concentrations obtained by filter analysis with extraction at pH 4.5. The dashed yellow line represents the concentrations from 1-min-filter
 420 extraction at pH 4.5. The dashed orange line represents the concentrations after 10-min-filter extraction at pH 4.5. The black dashed line
 represents the LOQ from blank measurements.

Table 3: Offline ws-Fe(II) and total ws-Fe concentrations from filter extraction. Filters were extracted for 1 h in pure Seradest water with pH 6.5 and with Seradest water adjusted to pH 4.5


ID	Location	Date	ws-Fe(II)	total ws-Fe	ws-Fe(II)/ total ws-Fe	ws-Fe(II)	total ws-Fe	ws-Fe(II)/ total ws-Fe	ws-Fe(II) _{pH 4.5} / ws-Fe(II) _{pH 6.5}	total ws-Fe _{pH 4.5} / total ws-Fe _{pH 6.5}
			[ng/m ⁻³] pH 6.5	[ng/m ⁻³] pH 6.5	[-] pH 6.5	[ng/m ⁻³] pH 4.5	[ng/m ⁻³] pH 4.5	[-] pH 4.5	pH 4.5/pH6.5	pH 4.5/pH6.5
A1	Berlin, Str. 17. J	04.06.-05.06.2024	10.1	18.5	0.5	n.a.	n.a.	n.a.	n.a.	n.a.
A2	Berlin, Str. 17. J	05.06.-06.06.2024	2.9	4.8	0.6	n.a.	n.a.	n.a.	n.a.	n.a.
A3	Berlin, Str. 17. J	06.06.-07.06.2024	8.7	10.7	0.	n.a.	n.a.	n.a.	n.a.	n.a.
A4	Berlin, Str. 17. J	07.06.-08.06.2024	17.0	23.1	0.72	n.a.	n.a.	n.a.	n.a.	n.a.
A5	Berlin, Str. 17. J	08.06.-09.06.2024	2.4	3.1	0.8	n.a.	n.a.	n.a.	n.a.	n.a.
B1	Berlin, TUB	03.06.-05.06.2024	5.1	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
B2	Berlin, TUB	05.06.-07.06.2024	2.4	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
B3	Berlin, TUB	10.06.-12.06.2024	0.3	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
B4	Berlin, TUB	12.06.-14.06.2024	0.1	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
B5	Berlin, TUB	22.03.-23.03.2025	1.1	3.2	0.3	10.8	11.8	0.92	9.80	3.68
B6	Berlin, TUB	23.03.-24.03.2025	2.9	7.3	0.4	21.6	25.5	0.85	7.46	3.47
B7	Berlin, TUB	24.03.-25.03.2025	7.5	16.5	0.5	34.5	41.5	0.83	4.60	2.52
B8	Berlin, TUB	25.03.-26.03.2025	5.5	18.2	0.2	17.4	25.5	0.68	3.16	1.03
C1	MH, Ireland	16.10-23.10.2024	< LOQ	< LOQ	n.a.	0.07	0.23	0.29	n.a.	n.a.
C2	MH, Ireland	14.11.-19.11.2024	0.04	0.06	0.81	0.13	0.29	0.45	2.9	5.2
C3	MH, Ireland	19.11.-27.11.2024	0.03	0.04	0.79	0.09	0.16	0.57	2.7	3.8
C4	MH, Ireland	27.11.-05.12.2024	0.02	0.03	0.80	0.07	0.13	0.50	2.7	4.2
C5	MH, Ireland	10.12.-19.12.2024	0.04	0.05	0.80	0.16	0.24	0.70	4.4	5.1

n.a.: no data available

On 09.06.2024, ws-Fe(II) concentrations decreased rapidly to values below the limit of quantification. Filter-based ws-Fe(II) was 2.4 ng m⁻³ (Table 3, Filter A5), while the online MARS-FIA system measured an average of 5.0 ng m⁻³. These results demonstrate a good agreement between online and offline measurements. The total ws-Fe concentrations for 08.06.2024 and 09.06.2024, determined from filter analysis, 23.1 ng m⁻³ and 3.1 ng m⁻³, respectively (Table 3, Filter A4 & A5), while average total ws-Fe concentrations from the online MARS-FIA system were higher, i.e. 31.7 ng m⁻³ and 7.6 ng m⁻³, respectively. The total ws-Fe concentrations measured by MARS-FIA are thus substantially higher compared to the filter analysis. Both, dissolved Fe(II) and Fe(III) ions are not stable in water at pH 6.5. On the one hand, dissolved Fe(II) quickly oxidizes to Fe(III). Pham and Waite (2008) found a half-life time for the oxidation of 50 nM dissolved Fe(II) of approximately 5 h at pH 6, which increases with increasing pH. Furthermore, dissolved Fe(III) rapidly hydrolyses to form Fe(OH)²⁺ and can subsequently undergo further hydrolysis and precipitation. Extraction for 1 h in Seradest water at pH 6.5 may therefore result in both oxidation of dissolved Fe(II) and hydrolysis and precipitation of Fe(III). Potentially, this could result in an insufficient reduction time of HA in the FIA system to fully reduce already hydrolysed Fe(III) back to Fe(II) as it was observed with aged Fe(III) standards (see section 3.1.1), leading to lower measured total ws-Fe concentrations compared to the online MARS-FIA system, where the sample is analysed within minutes and therefore less oxidation, hydrolysis and precipitation can be expected. The temporal variability of ws-Fe(II) and total ws-Fe concentrations during the field campaign with the PILS-FIA setup at the Campus of TU Berlin is illustrated in Figure 4b. The concentration of total ws-Fe ranges between 1.0 and 17.7 ng m⁻³ and thus not higher compared to the first field campaign even though the sample flow of the PILS-FIA setup was acidified to pH 4.5 (see section 2.2.1). In the period of 22.03. to 26.03.2025, 24 h-filters were collected (Table 3, Filters B5-8). To match the pH of extraction solution and wash flow from PILS, the filters were extracted at pH 4.5 and extracted with different extraction

times (see section 2.4.2). The shaded areas represent the concentrations determined for 1h-extraction time at pH 4.5. As highlighted in Figure 4b, the concentrations for both ws-Fe(II) and total ws-Fe determined are more than twice as high as those determined by the online PILS-FIA. A comparison of the concentration measured by PILS-FIA with those from the filters extracted for 1 min (yellow dashed line) and 10 min (orange dashed line, Figure 4b) shows that 1-minute extraction concentrations are lower than the online concentrations, while those after 10 min extraction fit well with concentrations determined with the online PILS-FIA setup. Due to missing PILS-FIA data from the evening of 24.03.2025 until the morning of 26.03.2025, only two filters (B5 & B8) can be compared with the online concentrations. The average concentrations determined with the PILS-FIA during the sampling period of filter B5 and B8 were 6.0 ngm^{-3} and 10.6 ngm^{-3} , respectively. When comparing these concentrations with the concentrations after 1, 5, 10 and 30 min of extraction (Table A2), the concentrations after 10 min of extraction, i.e. 6.0 and 13.9 ngm^{-3} , respectively, show very good agreement with the PILS-FIA measurement where the total residence time of the sample is around 15 min and 30 s (see section 3.1.2).

The ratio between ws-Fe(II) and total ws-Fe of the online system in relation to the total ws-Fe concentrations $> 5 \text{ ngm}^{-3}$ is shown in Figure 5. Total ws-Fe concentrations $> 5 \text{ ngm}^{-3}$ were chosen due to an increased relative error when calculating the ratios for lower total ws-Fe and ws-Fe(II) concentrations. The ratios during the summer test campaign with the MARS-FIA vary between mostly 0.5 and 0.7 resulting in an arithmetic mean of 0.66 and a median of 0.62 (Figure 5a).

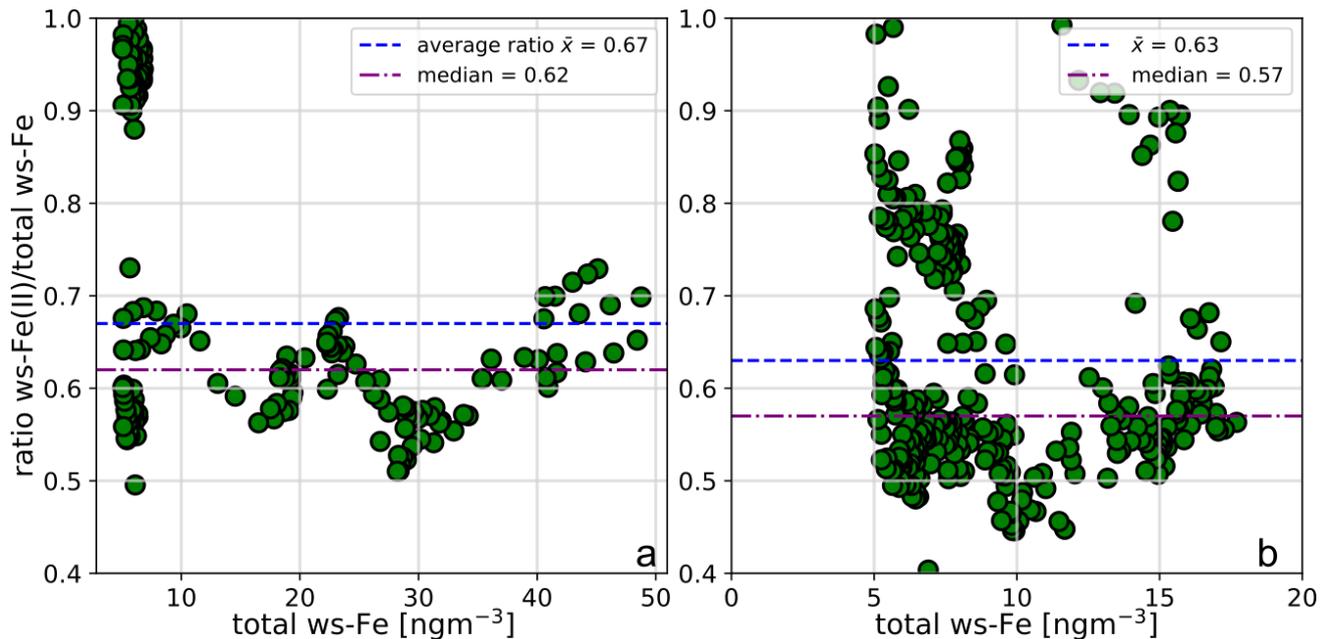

460

Figure 5: Ratios of ws-Fe(II)/total ws-Fe concentration over total ws-Fe concentration $> 5 \text{ ngm}^{-3}$ during a) the MARS field test campaign at *Straße des 17. Juni* in June 2024 and b) the PILS field test campaign on the campus of TU Berlin in March 2025.

465 The ratios during the winter test campaign with the PILS-FIA show higher variability compared to the first MARS-FIA test
campaign ranging from 0.4 to 1.0 resulting in an arithmetic mean of 0.63 and a median of 0.57 (Figure 5b). The ws-Fe(II) to
total ws-Fe ratio of the filter samples is listed in Table 3. The ratios from filter analysis from the MARS-FIA vary between
0.55 and 0.81 resulting in an arithmetic mean of 0.69, thus being slightly higher compared to the ratios determined with the
online system. The higher ws-Fe(II) to total ws-Fe ratios from the filter samples compared to the ratio determined by MARS-
470 FIA again reflect lower concentrations of total ws-Fe in offline filter analysis compared to the online system as discussed
above.

The arithmetic mean of the ratios of the four filters from the PILS-FIA test campaign, which were extracted at pH4.5 for 1 h,
is 0.82 and thus significantly higher compared to the mean ratio determined from the PILS-FIA online concentrations, which
is 0.63 and thus similar to the first test campaign (MARS-FIA with Seradest). While the ratios between the first and second
475 field campaigns determined online were similar, even though they were conducted at different extraction pH, the ratios ws-
Fe(II)/total ws-Fe from the filter extractions differ markedly between the two campaigns. The filter ratio from the first
campaign (extracted with Seradest water at pH 6.5) is 0.61, while that from the second campaign (extracted at pH 4.5) is 0.82.
This difference, comparable online ratios versus divergent offline ratios, highlights the influence of extraction time within the
online system, which appears to have a higher impact than acidification of the sample flow.

480 In general, no temporal difference in the ratios observed during day and night could be identified (see Figure A1). In a study
by Majestic et al. (2006) filter samples from an urban station in St. Louis (August 2004) were extracted with different leachates,
and the ws-Fe(II) and total ws-Fe concentrations were determined using the ferrozine method. In their study, ws-Fe
concentrations ranged from 5 to 25 ng m⁻³, depending on the leachate used, resulting in ws-Fe(II) to total ws-Fe ratios of 0.5
to 0.6. The ws-Fe(II) and total ws-Fe concentrations determined by both the MARS- and PILS-FIA setups in this study are
485 therefore consistent with previous work on ws-Fe in urban environments.

3.2.2 Comparison of ws-Fe With PM_{2.5} and Black Carbon (BC)

During the first field campaign in June 2024, the MARS-FIA setup was placed close to the main artery *road Straße des 17.
Juni* in Berlin city centre, thus measuring air which is highly influenced by traffic. Particle size distributions and BC
concentrations were also measured (see section 2.4.1). The temporal variability of PM_{2.5} (light-blue) and total ws-Fe (dark red)
490 is illustrated in Figure 6a. The PM_{2.5} concentrations varied between 2 and 47 µg m⁻³ resulting in an average of 14 µg m⁻³. The
total ws-Fe concentrations were three orders of magnitude lower, following the trend of the PM_{2.5} concentrations. Between
07.06. and 08.06.2024 the PM_{2.5} concentration remained relatively high around 30 µg m⁻³. Data for the 07.06.2024 are missing
from the PILS-FIA system but the highest total ws-Fe concentrations measured during the period were between 40 and
50 ng m⁻³ on 08.06.2024. reaching a maximum with 48.7 ng m⁻³ when also PM_{2.5} concentrations were high.

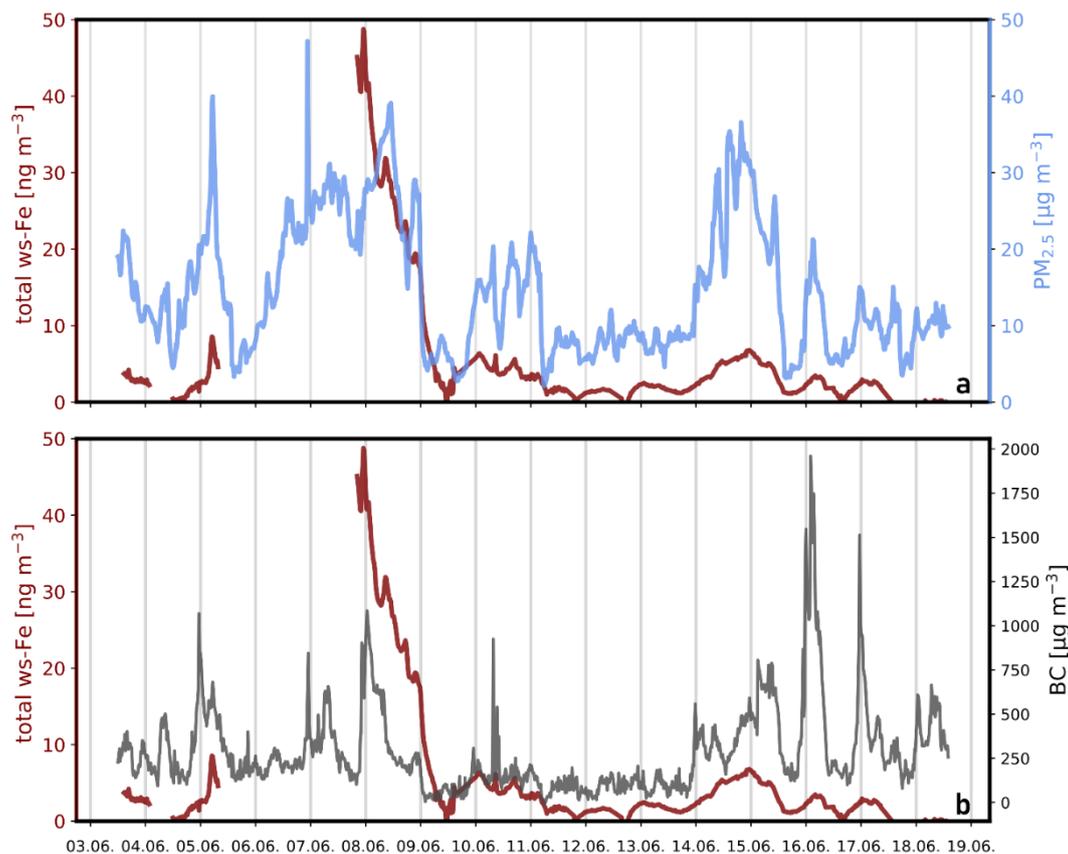


Figure 6: Temporal variability of total ws-Fe and PM_{2.5} (a) and total ws-Fe and BC(b) during the first test campaign at *Straße des 17. Juni* in June 2024.

In the night of 09.06.2024 both concentrations dropped rapidly, before they rose again on 10.06.2024. On 14.06.2024, PM_{2.5} again reached concentrations close to 40 µg m⁻³. Total ws-Fe concentrations also increase during that time reaching a maximum of 6.8 ng m⁻³ at 23:20 of 14.06.2024. For the linear regression between PM_{2.5} and total ws-Fe concentrations, a Pearson correlation coefficient of 0.49 indicates a moderate correlation ($p < 3.4 \cdot 10^{-47}$). Plotting the PM_{2.5} concentration against the total ws-Fe concentration (Figure 7a), two distinct groups of data points appear to form. The total ws-Fe concentrations higher than 15 ng m⁻³, measured on 08.06.2024 and highlighted in beige in Figure 7a, stand apart from the total ws-Fe concentrations below 15 ng m⁻³ from the rest of the campaign, shown in brown colour. Focusing on the lower total ws-Fe concentrations (< 15 ng m⁻³) in Figure 7b, these values correspond to a mass fraction of total ws-Fe between 0.15 and 2 % of PM_{2.5}, with most mass fractions falling between 0.15 and 0.3%. Contrary to the low total ws-Fe concentrations, the high total ws-Fe concentrations (>15 ng m⁻³) converge at a mass fraction of 2% of PM_{2.5}.

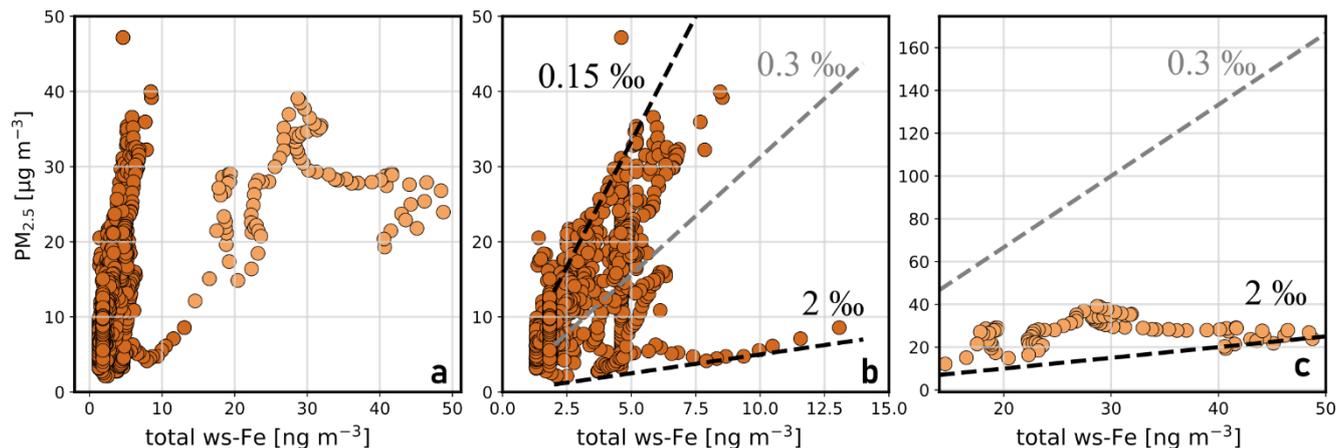


Figure 7: Relationship between $PM_{2.5}$ concentration and total ws-Fe concentration from the MARS-FIA test campaign in June 2024. (a) Scatter plot of all data points. $PM_{2.5}$ concentrations where the corresponding total ws-Fe concentration is $< 15 \text{ ng m}^{-3}$ are shown in brown. Those where the corresponding total ws-Fe concentration is $> 15 \text{ ng m}^{-3}$ are presented in beige. (b) Scatter plot of $PM_{2.5}$ versus total ws-Fe concentration $< 15 \text{ ng m}^{-3}$. The dashed lines correspond to Fe mass fractions of 2 ‰, 0.3 ‰ and 0.15 ‰, illustrating the range of mass fractions of ws-Fe in $PM_{2.5}$ observed during the campaign. (c) Scatter plot of $PM_{2.5}$ versus total ws-Fe concentration $> 15 \text{ ng m}^{-3}$, illustrating the mass fraction of total ws-Fe in $PM_{2.5}$ tends towards 2 ‰ for these concentration levels. Note the different scales in 7 (c).

515

Salazar et al. (2020a) reported an average water-soluble iron concentration of 7.7 ng m^{-3} in downtown Denver aerosols sampled during both summer and winter, corresponding to an average water-soluble iron fraction of approximately 4.2% of total iron. Crazzolaro and Held (2024) measured a contribution of total iron in PM_{10} ranging from 1.4 to 3.7% during a one-day measurement campaign in Berlin city centre. Assuming a total iron content of 1–4% in $PM_{2.5}$ and an iron solubility of 3–5%, the expected total ws-Fe concentration would range from approximately 0.3 to 2‰ of the total $PM_{2.5}$ mass. This is consistent with our measurements and evidences the plausibility of the data. The elevated concentrations on 08.06.2024 may either reflect generally high total iron levels or indicate an emission event specifically rich in water-soluble iron.

520

The ratio between ws-Fe(II) and total ws-Fe on 08.06.2024 was 0.59, which is slightly lower compared to the arithmetic mean value of 0.67 in the campaign, indicating increased emissions of reducible Fe(III) compared to ws-Fe(II) on 08.06.2024.

525

The temporal variability of BC (grey) and total ws-Fe concentrations is illustrated in Figure 6b. The concentration of BC varies between LOD and $2 \mu\text{g m}^{-3}$ reaching its maximum on 16.06.2024. For the linear regression between BC and total ws-Fe concentrations, a Pearson correlation coefficient of 0.35 ($p < 1.87 \cdot 10^{-23}$) indicates a weaker correlation for BC compared to the $PM_{2.5}$ concentrations. On 08.06.2024, when total ws-Fe concentrations were high ($> 15 \text{ ng m}^{-3}$), BC concentrations were also

530

elevated (see Figure A2) indicating an emission event that could be related to combustion processes such as traffic. ws-Fe concentrations originating from vehicle exhaust were investigated by Salazar et al., 2020b. They demonstrated that ws-Fe is formed through the dissolution of iron in water mediated by specific organic compounds present in the exhaust. The authors proposed that anthropogenic ws-Fe mainly results from chelation with these organic compounds or their likely aqueous reaction products. In addition to organic compounds emitted directly from exhaust, common atmospheric ligands can enhance solubility, even under moderately acidic conditions (Chen and Grassian, 2013). Deprotonated ligands replace surface OH

535

groups, thus forming a bidentate surface complex, which destabilizes the Fe-O bond (Wang et al., 2017). The formation of organic ligand-Fe complexes in the aqueous phase enhances further Fe dissolution from the aerosol into the liquid water phase (Sakata et al., 2022). Oxalate, which is ubiquitously present in aerosol particles, is considered an important complexing ligand alongside formate and acetate. Recently, oxalate has been observed in aged dust particles, which can enhance dissolution (Li et al., 2025). The complexation of Fe(III) by such ligands can additionally promote the photo-reduction to Fe(II) (Shi et al., 2012). Increased solubility in fog samples in the presence of metal-organic complexes has, for example, been observed by Giorio et al. (2025).

The second field campaign was conducted in March 2025 on the TU Berlin campus with the PILS-FIA setup with a sample flow pH of 4.5. During this period, air quality in Berlin ranged from moderate to poor, as indicated by PM_{2.5} concentrations at the Berlin background stations, which ranged up to 40 µg m⁻³ and averaged 20 µg m⁻³ over nine days (see Figure A3). In contrast, the average PM_{2.5} concentration during the first field campaign was only 8 µg m⁻³. The mean total ws-Fe concentration was 7.0 n g m⁻³, marginally higher than in the first campaign. Additionally, the variability in total ws-Fe concentrations was lower than previously observed, ranging from 2.7 to 17.2 ng m⁻³. The temporal patterns of both total ws-Fe (dark red) and PM_{2.5} (light blue), as well as total ws-Fe and black carbon (BC) concentrations (grey), are shown in Figure A4. As in the first field campaign, total ws-Fe trends followed both the PM_{2.5} and BC concentrations. The ratio of total ws-Fe to PM_{2.5} was consistent with the first campaign, ranging between 0.15 and 2 ‰ (see Figure A4a). The Pearson correlation coefficient between total ws-Fe concentrations >5 ng m⁻³ and PM_{2.5} was 0.25 (p < 0.004), indicating a weak correlation. Similarly, a weak correlation was observed between total ws-Fe concentrations >5 ng m⁻³ and BC concentrations <800 µg m⁻³ (Pearson r = 0.28, p < 1.6×10⁻⁵). The average ratio of ws-Fe(II) to total ws-Fe for concentrations above 5 ng m⁻³ was 0.63, only slightly lower than in the first campaign (see Figure 5).

Overall, the second campaign, conducted in winter 2025 at the campus of TU Berlin, showed total ws-Fe concentrations comparable to the first campaign in summer (June 2024 at *Straße des 17. Juni*) thus indicating no clear seasonal difference even though the PM_{2.5} concentrations of the background stations were notably higher during the winter test campaign. Salazar et al. (2020a) investigated ws-Fe concentrations at three locations, which were defined as 1) urban, 2) rural and agriculture and 3) urban and agriculture in summer and winter of 2016 and 2017. Across all three sites they observed that ws-Fe concentrations were lower in winter, even though total iron concentrations were higher during that season. Similarly, Ye et al. (2018) analysed long-term filter samples collected in Atlanta from 1998 to 2013 and found that seasonal and long-term trends in ws-Fe closely followed sulfate concentrations, which were elevated in summer and showed a long-term decline attributed to reduced coal combustion. Based on the same data set, Wong et al. (2020) further concluded that sulfate promotes acidic aerosol conditions and particle water that enhance the dissolution of iron, with ws-Fe variability mainly controlled by particle liquid water and stronger effects in summer, while combustion sources contribute relatively more in winter.

In Europe, sulfate concentrations have decreased by approximately 0.15 µg yr⁻¹ between 2000 and 2018 (Tsimpidi et al., 2025). This long-term decline likely contributes to the generally lower ws-Fe concentrations observed during the Berlin campaigns compared to those reported for Atlanta between 2008 and 2013 (average 24.22 ng m⁻³, Ye et al., 2018). Nevertheless, ws-Fe

570 concentrations measured during one week in March 2025 and during nearly three weeks in June 2025 were comparable, despite representing different seasons.

The absence of a clear seasonal difference in the present study may partly result from comparing measurements at two-nearby sites but still differently influenced by traffic. Importantly, however, the results of the second test campaign underline that the slightly acidic wash flow of pH 4.5 used in the PILS-FIA setup does not significantly affect iron's solubility or oxidation state
575 during sampling compared to sampling in MARS with pH 6.5.

4. Suitability of the FIA System for Field Measurements

Both field test campaigns demonstrate that the developed FIA system, designed for near real-time measurement of ws-Fe(II) and total ws-Fe concentrations in particulate matter, can be effectively used in combination with the MARS and PILS sampling
580 units in an urban environment. The system is suitable for urban environments where total ws-Fe concentrations exceed 1 ng m^{-3} . To assess its applicability in different environmental conditions, filter samples were collected at Mace Head, Ireland, as described in section 2.3.2. Because Mace Head represents a pristine environment with expectedly low iron concentrations, filter sampling with a sampling periods between 5 and 10 days was performed. Results shown in Table 3 indicate very low total ws-Fe concentrations - ranging from <LOQ to 0.05 ng m^{-3} - when extracted with Seradest water at pH 6.5. These findings
585 illustrate the substantially lower iron solubility in regions with minimal anthropogenic emissions. Even after acidifying the extraction solution to pH 4.5 representing cloud-water relevant conditions, total ws-Fe concentrations ranged between 0.13-
0.29 ng m^{-3} , thus still remaining below 1 ng m^{-3} .

For application at remote sites with total ws-Fe concentrations below 1 ng m^{-3} , the LOQs of both the MARS-FIA and PILS-FIA setups, given their current settings, are too high to reliably detect near real-time ws-Fe concentrations. Further acidification
590 of the wash flow to pH 2 or 3 is unlikely to sufficiently boost water-soluble iron concentrations due to the short extraction times available. Therefore, quantification of ws-Fe in remote locations would require methodological adaptations, such as pre-concentration, increasing extraction time within the sampling unit, extending residence time in the online apparatus before ferrozine addition, or increasing the ratio of gas volume to volume of extractant through collecting larger air sample volumes. Nevertheless, the FIA system was successfully applied in two field campaigns in Berlin, and provides speciation capability of
595 water-soluble iron in ambient aerosols in future field measurements, especially in urban and semi-urban environments.

Acknowledgements

We gratefully acknowledge funding from the ATMO-ACCESS project, which has received funding from the European Union's Horizon 2020 Research and Innovation Framework Programme (H2020-INFRAIA).

Access to the Mace Head Atmospheric Research Station for the FeNTASI project was provided through the ACTRIS Trans-
600 National Access (TNA) programme (project ID: ATMO-TNA-5G--0000000065). Further, we would like to thank Metrohm

Process Analytics for providing the MARS system and especially Kerstin Dreblow and Jerry van Bronckhorst for their invaluable support with the MARS system.

Author Contributions

605 S.L.: Conceptualization, Methodology, Software, Validation, Formal Analysis, Investigation, Writing-Original Draft, S.K:
Methodology, Conceptualization, Investigation, F.F.: Methodology, Software, D.C.: Investigation, Resources, Writing-
Review & Editing, D.v.P.: Resources, Writing-Review & Editing, H.H.: Resources, Writing-Review & Editing, W.F.:
Methodology, Conceptualization, Writing-Review & Editing, A.H.: Conceptualization, Software, Resources, Writing-Review
& Editing.

Competing interests

610 A.H. is a member of the editorial board of *Aerosol Research*.

615

620

625

630

Appendix

Table A1: Results of linear regression from calibration over one year

Date	a	b	R ²	pH
08.04.2024	0.0244	-0.0050	0.9997	6.5
09.04.2024	0.0255	-0.0019	0.9955	6.5
11.04.2024	0.0246	-0.0015	0.9977	6.5
14.02.2024	0.0224	-0.0014	0.9951	6.5
28.05.2024	0.0252	-0.0193	0.9983	6.5
10.11.2024	0.0222	-0.0025	0.9999	3.5
13.02.2025	0.0206	-0.0036	0.9918	3.5
18.02.2025	0.028	-0.001	0.9998	3.5
27.05.2025	0.0269	0.0119	0.99	6.5
04.06.2025	0.0218	0.0009	0.99	6.5

635 **Table A2:** Total ws-Fe concentration depending on extraction time in acidified water (pH 4.5)

	1 min	5 min	10 min	30 min
Filter B5 22.-23.03.2025: Total ws-Fe [ng m ⁻³]	2.1	4.1	6.0	22.7
Filter B6 23.-24.03.2025: Total ws-Fe [ng m ⁻³]	4.01	6.9	11.5	18.5
Filter B7 24.-25.03.2025: Total ws-Fe [ng m ⁻³]	14.1	17.5	26.7	24.6
Filter B8 25.-26.03.2025: Total ws-Fe [ng m ⁻³]	5.7	7.0	13.9	18.2



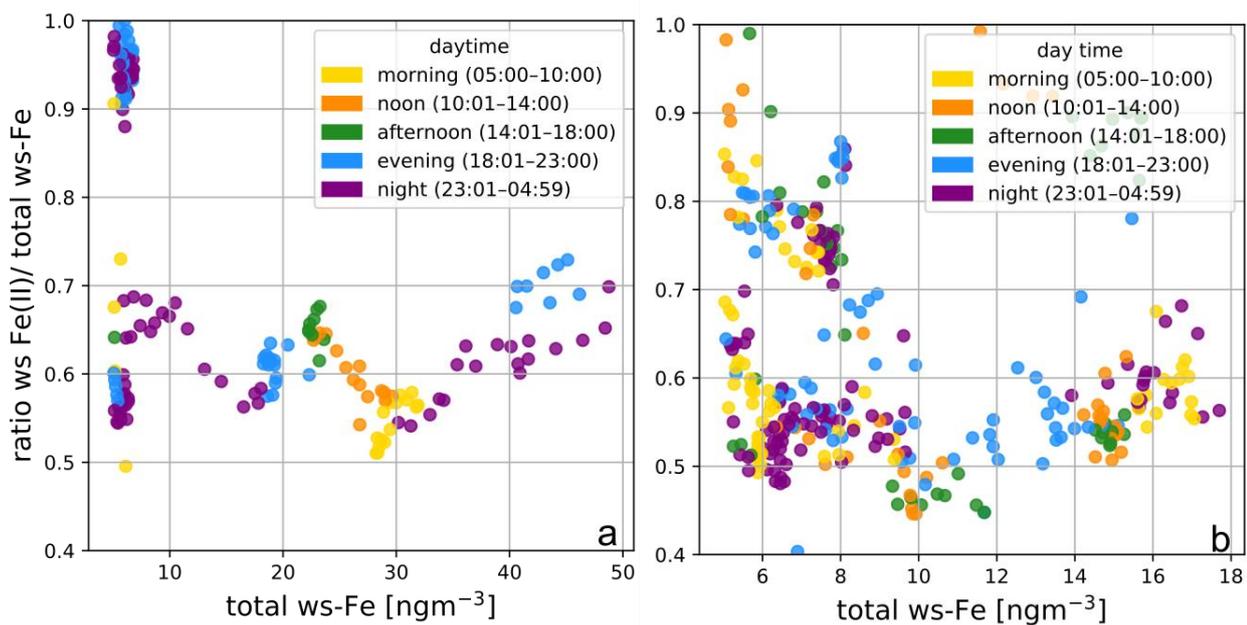



Figure A1: Ratios of ws-Fe(II) to total ws-Fe over total ws-Fe concentration $> 5\text{ngm}^{-3}$ coloured depending on time of the day at a) Straße des 17. Juni and b) on the campus of TU Berlin

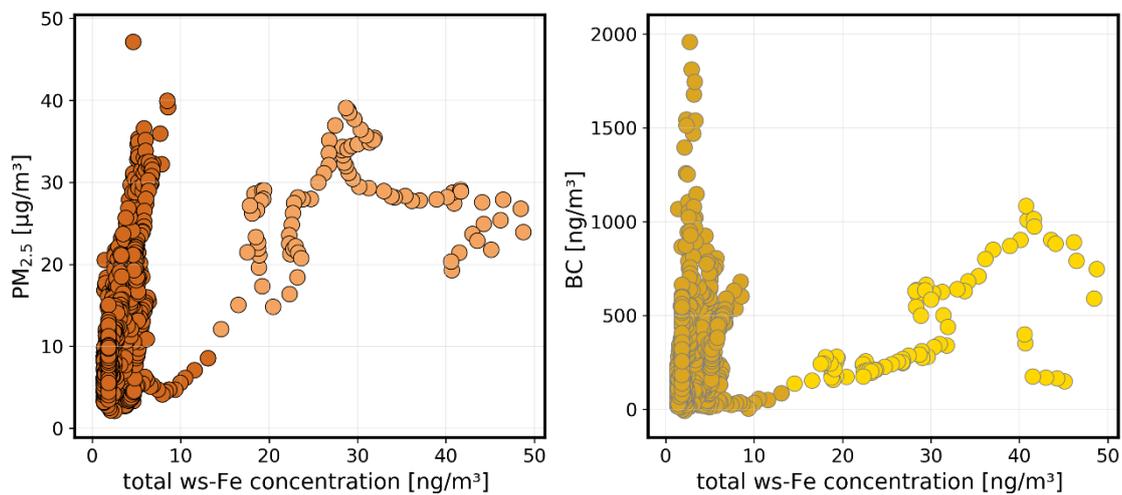

640 Figure A2: Total ws-Fe concentration to PM_{2.5} concentrations (left) and BC concentrations (right)

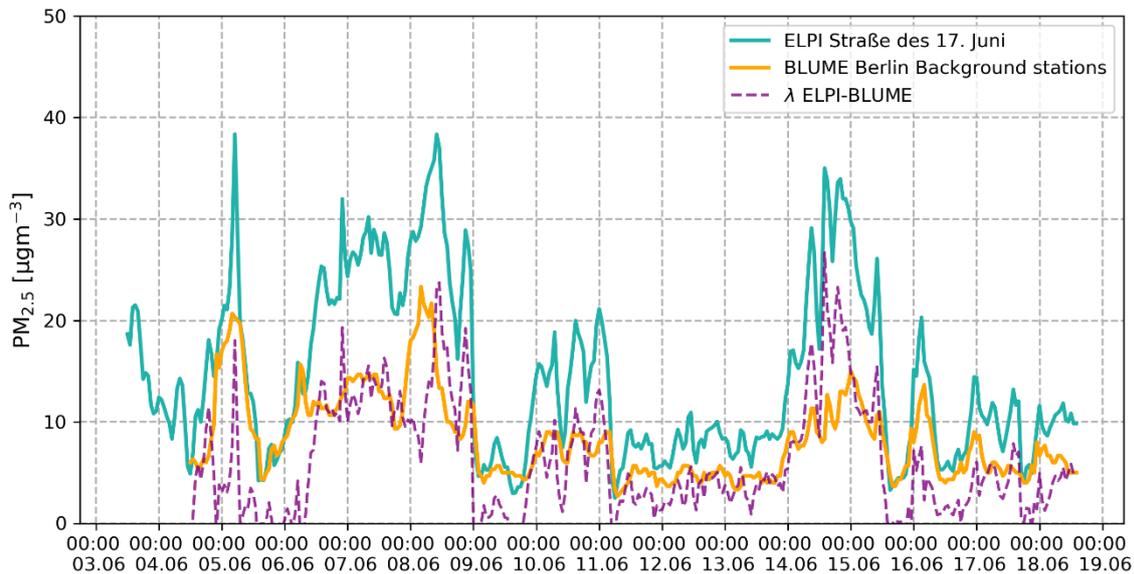

645 **Figure A3: Temporal variability of PM_{2.5} concentrations** at Straße des 17. Juni (turquoise) and average concentrations from background stations Neukölln, Mitte and Wedding from Berlin BLUME air quality network (yellow). The purple dashed lines represent the difference between the ELPI measurements at Straße des 17. Juni and the averaged concentrations from BLUME air quality network.

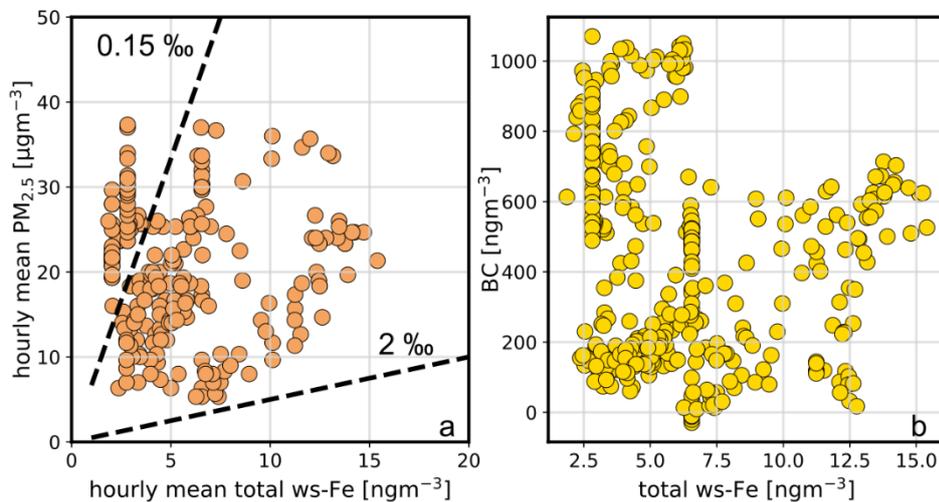

650 **Figure A4: Hourly averaged PM_{2.5} concentration from BLUME background stations over hourly averaged total ws-Fe concentration (a) and BC concentration over total ws-Fe concentrations (b).**

References

- Al-Abadleh, H. A.: Iron content in aerosol particles and its impact on atmospheric chemistry, *Chem. Commun.*, 60, 1840–1855, <https://doi.org/10.1039/D3CC04614A>, 2024.
- 655 Al-Abadleh, H. A., Smith, M., Ogilvie, A., and Sadiq, N. W.: Quantifying the Effect of Basic Minerals on Acid- and Ligand-Promoted Dissolution Kinetics of Iron in Simulated Dark Atmospheric Aging of Dust and Coal Fly Ash Particles, *J. Phys. Chem. A*, 128, 8198–8208, <https://doi.org/10.1021/acs.jpca.4c05181>, 2024.
- Arakaki, T. and Faust, B. C.: Sources, sinks, and mechanisms of hydroxyl radical ($\bullet\text{OH}$) photoproduction and consumption in authentic acidic continental cloud waters from Whiteface Mountain, New York: The role of the Fe(r) (r = II, III) photochemical cycle, *Journal of Geophysical Research: Atmospheres*, 103, 3487–3504, <https://doi.org/10.1029/97JD02795>, 1998.
- 660 Attiyat, A. S., Al-Momani, I. F., and Moussa, M. A.: Simultaneous Spectrophotometric Determination of Iron (II) and Total Iron Using Flow Injection Analysis, *ABHATH AL-YARMOUK*, 67, 2011.
- Baldo, C., Ito, A., Krom, M. D., Li, W., Jones, T., Drake, N., Ignatyev, K., Davidson, N., and Shi, Z.: Iron from coal combustion particles dissolves much faster than mineral dust under simulated atmospheric acidic conditions, *Atmospheric Chemistry and Physics*, 22, 6045–6066, <https://doi.org/10.5194/acp-22-6045-2022>, 2022.
- 665 Balsamo Crespo, E., Reichelt-Brushett, A., Smith, R. E. W., Rose, A. L., and Batley, G. E.: Improving the Measurement of Iron(III) Bioavailability in Freshwater Samples: Methods and Performance, *Environ Toxicol Chem*, 42, 303–316, <https://doi.org/10.1002/etc.5530>, 2023.
- Bianco, A., Passananti, M., Brigante, M., and Mailhot, G.: Photochemistry of the Cloud Aqueous Phase: A Review, *Molecules*, 670 25, 423, <https://doi.org/10.3390/molecules25020423>, 2020.
- Browning, T. J. and Moore, C. M.: Global analysis of ocean phytoplankton nutrient limitation reveals high prevalence of co-limitation, *Nat Commun*, 14, 5014, <https://doi.org/10.1038/s41467-023-40774-0>, 2023.
- Chen, H. and Grassian, V. H.: Iron Dissolution of Dust Source Materials during Simulated Acidic Processing: The Effect of Sulfuric, Acetic, and Oxalic Acids, *Environ. Sci. Technol.*, 47, 10312–10321, <https://doi.org/10.1021/es401285s>, 2013.
- 675 Chen, Y. and Siefert, R. L.: Determination of various types of labile atmospheric iron over remote oceans, *Journal of Geophysical Research: Atmospheres*, 108, <https://doi.org/10.1029/2003JD003515>, 2003.
- Chu, B., Liggio, J., Liu, Y., He, H., Takekawa, H., Li, S.-M., and Hao, J.: Influence of metal-mediated aerosol-phase oxidation on secondary organic aerosol formation from the ozonolysis and OH-oxidation of α -pinene, *Sci Rep*, 7, 40311, <https://doi.org/10.1038/srep40311>, 2017.
- 680 Crazzolara, C. and Held, A.: Development of a cascade impactor optimized for size-fractionated analysis of aerosol metal content by total reflection X-ray fluorescence spectroscopy (TXRF), *Atmospheric Measurement Techniques*, 17, 2183–2194, <https://doi.org/10.5194/amt-17-2183-2024>, 2024.
- 685 De Haan, D. O., Hawkins, L. N., Weber, J. A., Moul, B. T., Hui, S., Cox, S. A., Esse, J. U., Skochdopole, N. R., Lynch, C. P., De Haan, A. C., Le, C., Cazaunau, M., Bergé, A., Pangui, E., Heuser, J., Doussin, J.-F., and Picquet-Varrault, B.: Brown Carbon Aerosol Formation by Multiphase Catechol Photooxidation in the Presence of Soluble Iron, *ACS EST Air*, 1, 909–917, <https://doi.org/10.1021/acsestair.4c00045>, 2024.

- Deguillaume, L., Leriche, M., Desboeufs, K., Mailhot, G., George, C., and Chaumerliac, N.: Transition Metals in Atmospheric Liquid Phases: Sources, Reactivity, and Sensitive Parameters, *Chem. Rev.*, 105, 3388–3431, <https://doi.org/10.1021/cr040649c>, 2005.
- 690 Fan, S.-M., Moxim, W. J., and Levy II, H.: Aeolian input of bioavailable iron to the ocean, *Geophysical Research Letters*, 33, <https://doi.org/10.1029/2005GL024852>, 2006.
- Fenton, H. J. J.: Oxidation of tartaric acid in presence... - Google Scholar, *Journal of the Chemical Society, Transactions*, 899–910, 1894.
- 695 Fu, H., Lin, J., Shang, G., Dong, W., Grassian, V. H., Carmichael, G. R., Li, Y., and Chen, J.: Solubility of Iron from Combustion Source Particles in Acidic Media Linked to Iron Speciation, *Environ. Sci. Technol.*, 46, 11119–11127, <https://doi.org/10.1021/es302558m>, 2012.
- Gao, Y., Marsay, C. M., Yu, S., Fan, S., Mukherjee, P., Buck, C. S., and Landing, W. M.: Particle-Size Variability of Aerosol Iron and Impact on Iron Solubility and Dry Deposition Fluxes to the Arctic Ocean, *Sci Rep*, 9, 16653, <https://doi.org/10.1038/s41598-019-52468-z>, 2019.
- 700 Gao, Y., Yu, S., Sherrell, R. M., Fan, S., Bu, K., and Anderson, J. R.: Particle-Size Distributions and Solubility of Aerosol Iron Over the Antarctic Peninsula During Austral Summer, *Journal of Geophysical Research: Atmospheres*, 125, e2019JD032082, <https://doi.org/10.1029/2019JD032082>, 2020.
- Giorio, C., Borca, C. N., Zhrebker, A., D’Aronco, S., Saidikova, M., Sheikh, H. A., Harrison, R. J., Badocco, D., Soldà, L., Pastore, P., Ammann, M., and Huthwelker, T.: Iron Speciation in Urban Atmospheric Aerosols: Comparison between Thermodynamic Modeling and Direct Measurements, *ACS Earth Space Chem.*, 9, 649–661, <https://doi.org/10.1021/acsearthspacechem.4c00359>, 2025.
- Herrmann, H., Schaefer, T., Tilgner, A., Styler, S. A., Weller, C., Teich, M., and Otto, T.: Tropospheric Aqueous-Phase Chemistry: Kinetics, Mechanisms, and Its Coupling to a Changing Gas Phase, *Chem. Rev.*, 115, 4259–4334, <https://doi.org/10.1021/cr500447k>, 2015.
- 710 Hopstock, K. S., Carpenter, B. P., Patterson, J. P., Al-Abadleh, H. A., and Nizkorodov, S. A.: Formation of insoluble brown carbon through iron-catalyzed reaction of biomass burning organics, *Environmental Science: Atmospheres*, 3, 207–220, 2023.
- Hutchins, D. A. and Tagliabue, A.: Feedbacks between phytoplankton and nutrient cycles in a warming ocean, *Nat. Geosci.*, 17, 495–502, <https://doi.org/10.1038/s41561-024-01454-w>, 2024.
- 715 Ito, A.: Atmospheric Processing of Combustion Aerosols as a Source of Bioavailable Iron, *Environ. Sci. Technol. Lett.*, 2, 70–75, <https://doi.org/10.1021/acs.estlett.5b00007>, 2015.
- Ito, A. and Shi, Z.: Delivery of anthropogenic bioavailable iron from mineral dust and combustion aerosols to the ocean, *Atmospheric Chemistry and Physics*, 16, 85–99, <https://doi.org/10.5194/acp-16-85-2016>, 2016.
- 720 Ito, A., Myriokefalitakis, S., Kanakidou, M., Mahowald, N. M., Scanza, R. A., Hamilton, D. S., Baker, A. R., Jickells, T., Sarin, M., Bikkina, S., Gao, Y., Shelley, R. U., Buck, C. S., Landing, W. M., Bowie, A. R., Perron, M. M. G., Guieu, C., Meskhidze, N., Johnson, M. S., Feng, Y., Kok, J. F., Nenes, A., and Duce, R. A.: Pyrogenic iron: The missing link to high iron solubility in aerosols, *Science Advances*, 5, eaau7671, <https://doi.org/10.1126/sciadv.aau7671>, 2019.
- Jickells, T. D., An, Z. S., Andersen, K. K., Baker, A. R., Bergametti, G., Brooks, N., Cao, J. J., Boyd, P. W., Duce, R. A., Hunter, K. A., Kawahata, H., Kubilay, N., laRoche, J., Liss, P. S., Mahowald, N., Prospero, J. M., Ridgwell, A. J., Tegen, I.,

- and Torres, R.: Global Iron Connections Between Desert Dust, Ocean Biogeochemistry, and Climate, *Science*, 308, 67–71, 725 <https://doi.org/10.1126/science.1105959>, 2005.
- Journet, E., Desboeufs, K. V., Caquineau, S., and Colin, J.-L.: Mineralogy as a critical factor of dust iron solubility, *Geophysical Research Letters*, 35, <https://doi.org/10.1029/2007GL031589>, 2008.
- Kieber, R. J., Skrabal, S. A., Smith, B. J., and Willey, J. D.: Organic Complexation of Fe(II) and Its Impact on the Redox Cycling of Iron in Rain, *Environ. Sci. Technol.*, 39, 1576–1583, <https://doi.org/10.1021/es040439h>, 2005.
- 730 Kuang, X. M., Scott, John A., da Rocha, Gisele O., Betha, Raghu, Price, Derek J., Russell, Lynn M., Cocker, David R., and Paulson, S. E.: Hydroxyl radical formation and soluble trace metal content in particulate matter from renewable diesel and ultra low sulfur diesel in at-sea operations of a research vessel, *Aerosol Science and Technology*, 51, 147–158, <https://doi.org/10.1080/02786826.2016.1271938>, 2017.
- 735 Kuang, X. M., Gonzalez, D. H., Scott, J. A., Vu, K., Hasson, A., Charbouillot, T., Hawkins, L., and Paulson, S. E.: Cloud Water Chemistry Associated with Urban Aerosols: Rapid Hydroxyl Radical Formation, Soluble Metals, Fe(II), Fe(III), and Quinones, *ACS Earth Space Chem.*, 4, 67–76, <https://doi.org/10.1021/acsearthspacechem.9b00243>, 2020.
- Langmuir, D.: *Aqueous environmental geochemistry*, New Jersey, 1997.
- Lei, Y., Li, D., Lu, D., Zhang, T., Sun, J., Wang, X., Xu, H., and Shen, Z.: Insights into the roles of aerosol soluble iron in secondary aerosol formation, *Atmospheric Environment*, 294, 119507, <https://doi.org/10.1016/j.atmosenv.2022.119507>, 2023.
- 740 Li, R., Dong, S., Huang, C., Yu, F., Wang, F., Li, X., Zhang, H., Ren, Y., Guo, M., Chen, Q., Ge, B., and Tang, M.: Evaluating the effects of contact time and leaching solution on measured solubilities of aerosol trace metals, *Applied Geochemistry*, 148, 105551, <https://doi.org/10.1016/j.apgeochem.2022.105551>, 2023.
- Li, W., Qi, Y., Wu, G., Zhang, Y., Han, R., Liu, Y., Qu, W., Song, Y., Wang, X., Chen, T., Sheng, L., Shi, J., Zhang, D., and Zhou, Y.: Anthropogenic Dominance and Secondary Processes Drive Aerosol Iron Solubility in Asian Continental Outflow: 745 Insights from Spring Qingdao, China, *ACS EST Air*, 2, 1840–1848, <https://doi.org/10.1021/acsestair.5c00049>, 2025.
- Liu, L., Li, W., Lin, Q., Wang, Y., Zhang, J., Zhu, Y., Yuan, Q., Zhou, S., Zhang, D., Baldo, C., and Shi, Z.: Size-dependent aerosol iron solubility in an urban atmosphere, *npj Clim Atmos Sci*, 5, 53, <https://doi.org/10.1038/s41612-022-00277-z>, 2022.
- Liu, X. and Millero, F. J.: The solubility of iron hydroxide in sodium chloride solutions, *Geochimica et Cosmochimica Acta*, 63, 3487–3497, [https://doi.org/10.1016/S0016-7037\(99\)00270-7](https://doi.org/10.1016/S0016-7037(99)00270-7), 1999.
- 750 Liu, X. and Millero, F. J.: The solubility of iron in seawater, *Marine Chemistry*, 77, 43–54, [https://doi.org/10.1016/S0304-4203\(01\)00074-3](https://doi.org/10.1016/S0304-4203(01)00074-3), 2002.
- Longo, A. F., Feng, Y., Lai, B., Landing, W. M., Shelley, R. U., Nenes, A., Mihalopoulos, N., Violaki, K., and Ingall, E. D.: Influence of Atmospheric Processes on the Solubility and Composition of Iron in Saharan Dust, *Environ. Sci. Technol.*, 50, 6912–6920, <https://doi.org/10.1021/acs.est.6b02605>, 2016.
- 755 Lührtrath, S., Klemer, S., Dubois, C., George, C., and Held, A.: Impact of atmospheric water-soluble iron on α -pinene-derived SOA formation and transformation in the presence of aqueous droplets, *Environmental Science: Atmospheres*, 4, 1218–1228, <https://doi.org/10.1039/D4EA00095A>, 2024.

- Lüchtrath, S., Wutke, R., and Held, A.: Secondary Formation of Light-Absorbing, Insoluble Particles from Catechol in the Presence of Fe(II) or Fe(III) and Hydrogen Peroxide at Dark and Light Conditions, *ACS EST Air*, 760 <https://doi.org/10.1021/acsestair.5c00091>, 2025.
- Luo, C., Mahowald, N. M., Meskhidze, N., Chen, Y., Siefert, R. L., Baker, A. R., and Johansen, A. M.: Estimation of iron solubility from observations and a global aerosol model, *J. Geophys. Res.*, 110, 2005JD006059, <https://doi.org/10.1029/2005JD006059>, 2005.
- Luo, C., Mahowald, N., Bond, T., Chuang, P. Y., Artaxo, P., Siefert, R., Chen, Y., and Schauer, J.: Combustion iron distribution and deposition, *Global Biogeochemical Cycles*, 22, <https://doi.org/10.1029/2007GB002964>, 2008.
- Luther, G. W., Shellenbarger, P. A., and Brendel, P. J.: Dissolved organic Fe(III) and Fe(II) complexes in salt marsh porewaters, *Geochimica et Cosmochimica Acta*, 60, 951–960, [https://doi.org/10.1016/0016-7037\(95\)00444-0](https://doi.org/10.1016/0016-7037(95)00444-0), 1996.
- Ma, Y.: Developments and improvements to the particle-into-liquid sampler (PILS) and its application to Asian outflow studies, Georgia Institute of Technology, 2004.
- 770 Mahowald, N. M., Engelstaedter, S., Luo, C., Sealy, A., Artaxo, P., Benitez-Nelson, C., Bonnet, S., Chen, Y., Chuang, P. Y., Cohen, D. D., Dulac, F., Herut, B., Johansen, A. M., Kubilay, N., Losno, R., Maenhaut, W., Paytan, A., Prospero, J. M., Shank, L. M., and Siefert, R. L.: Atmospheric Iron Deposition: Global Distribution, Variability, and Human Perturbations*, *Annual Review of Marine Science*, 1, 245–278, <https://doi.org/10.1146/annurev.marine.010908.163727>, 2009.
- 775 Majestic, B. J., Schauer, J. J., Shafer, M. M., Turner, J. R., Fine, P. M., Singh, M., and Sioutas, C.: Development of a Wet-Chemical Method for the Speciation of Iron in Atmospheric Aerosols, *Environ. Sci. Technol.*, 40, 2346–2351, <https://doi.org/10.1021/es052023p>, 2006.
- Meskhidze, N., Johnson, M. S., Hurley, D., and Dawson, K.: Influence of measurement uncertainties on fractional solubility of iron in mineral aerosols over the oceans, *Aeolian Research*, 22, 85–92, <https://doi.org/10.1016/j.aeolia.2016.07.002>, 2016.
- 780 Meskhidze, N., Hurley, D., Royalty, T. M., and Johnson, M. S.: Potential effect of atmospheric dissolved organic carbon on the iron solubility in seawater, *Marine Chemistry*, 194, 124–132, <https://doi.org/10.1016/j.marchem.2017.05.011>, 2017.
- Millero, F. J., Sotolongo, S., and Izaguirre, M.: The oxidation kinetics of Fe(II) in seawater, *Geochimica et Cosmochimica Acta*, 51, 793–801, [https://doi.org/10.1016/0016-7037\(87\)90093-7](https://doi.org/10.1016/0016-7037(87)90093-7), 1987.
- 785 Moore, C. M., Mills, M. M., Arrigo, K. R., Berman-Frank, I., Bopp, L., Boyd, P. W., Galbraith, E. D., Geider, R. J., Guieu, C., Jaccard, S. L., Jickells, T. D., La Roche, J., Lenton, T. M., Mahowald, N. M., Marañón, E., Marinov, I., Moore, J. K., Nakatsuka, T., Oschlies, A., Saito, M. A., Thingstad, T. F., Tsuda, A., and Ulloa, O.: Processes and patterns of oceanic nutrient limitation, *Nature Geosci*, 6, 701–710, <https://doi.org/10.1038/ngeo1765>, 2013.
- Murray, J. W. and Gill, G.: The geochemistry of iron in puget sound, *Geochimica et Cosmochimica Acta*, 42, 9–19, [https://doi.org/10.1016/0016-7037\(78\)90211-9](https://doi.org/10.1016/0016-7037(78)90211-9), 1978.
- 790 Nagy, G., Fehér, Zs., and Pungor, E.: Application of silicone rubber-based graphite electrodes for continuous flow measurements: Part II. Voltammetric study of active substances injected into electrolyte streams, *Analytica Chimica Acta*, 52, 47–54, [https://doi.org/10.1016/S0003-2670\(01\)80040-4](https://doi.org/10.1016/S0003-2670(01)80040-4), 1970.
- Oakes, M., Rastogi, N., Majestic, B. J., Shafer, M., Schauer, J. J., Edgerton, E. S., and Weber, R. J.: Characterization of soluble iron in urban aerosols using near-real time data, *Journal of Geophysical Research: Atmospheres*, 115, <https://doi.org/10.1029/2009JD012532>, 2010.

- 795 O'Connor, T. C., Jennings, S. G., and O'Dowd, C. D.: Highlights of fifty years of atmospheric aerosol research at Mace Head, *Atmospheric Research*, 90, 338–355, <https://doi.org/10.1016/j.atmosres.2008.08.014>, 2008.
- Orsini, D. A., Ma, Y., Sullivan, A., Sierau, B., Baumann, K., and Weber, R. J.: Refinements to the particle-into-liquid sampler (PILS) for ground and airborne measurements of water soluble aerosol composition, *Atmospheric Environment*, 37, 1243–1259, [https://doi.org/10.1016/S1352-2310\(02\)01015-4](https://doi.org/10.1016/S1352-2310(02)01015-4), 2003.
- 800 Paris, R. and Desboeufs, K. V.: Effect of atmospheric organic complexation on iron-bearing dust solubility, *Atmospheric Chemistry and Physics*, 13, 4895–4905, <https://doi.org/10.5194/acp-13-4895-2013>, 2013.
- Pascual-Reguera, M. I., Ortega-Carmona, I., and Molina-Díaz, A.: Spectrophotometric determination of iron with ferrozine by flow-injection analysis, *Talanta*, 44, 1793–1801, [https://doi.org/10.1016/S0039-9140\(97\)00050-7](https://doi.org/10.1016/S0039-9140(97)00050-7), 1997.
- 805 Pehkonen, S. O., Siefert, R., Erel, Y., Webb, S., and Hoffmann, M. R.: Photoreduction of iron oxyhydroxides in the presence of important atmospheric organic compounds, *Environ. Sci. Technol.*, 27, 2056–2062, <https://doi.org/10.1021/es00047a010>, 1993.
- Perron, M. M. G., Strzelec, M., Gault-Ringold, M., Proemse, B. C., Boyd, P. W., and Bowie, A. R.: Assessment of leaching protocols to determine the solubility of trace metals in aerosols, *Talanta*, 208, 120377, <https://doi.org/10.1016/j.talanta.2019.120377>, 2020.
- 810 Pham, A. N. and Waite, T. D.: Oxygenation of Fe(II) in natural waters revisited: Kinetic modeling approaches, rate constant estimation and the importance of various reaction pathways, *Geochimica et Cosmochimica Acta*, 72, 3616–3630, <https://doi.org/10.1016/j.gca.2008.05.032>, 2008.
- Pullin, M. J. and Cabaniss, S. E.: Colorimetric flow-injection analysis of dissolved iron in high DOC waters, *Water Research*, 35, 363–372, [https://doi.org/10.1016/S0043-1354\(00\)00259-1](https://doi.org/10.1016/S0043-1354(00)00259-1), 2001.
- 815 Pye, H. O. T., Nenes, A., Alexander, B., Ault, A. P., Barth, M. C., Clegg, S. L., Collett Jr., J. L., Fahey, K. M., Hennigan, C. J., Herrmann, H., Kanakidou, M., Kelly, J. T., Ku, I.-T., McNeill, V. F., Riemer, N., Schaefer, T., Shi, G., Tilgner, A., Walker, J. T., Wang, T., Weber, R., Xing, J., Zaveri, R. A., and Zuend, A.: The acidity of atmospheric particles and clouds, *Atmospheric Chemistry and Physics*, 20, 4809–4888, <https://doi.org/10.5194/acp-20-4809-2020>, 2020.
- 820 Raiswell, R., Benning, L. G., Tranter, M., and Tulaczyk, S.: Bioavailable iron in the Southern Ocean: the significance of the iceberg conveyor belt, *Geochem Trans*, 9, 7, <https://doi.org/10.1186/1467-4866-9-7>, 2008.
- Rastogi, N., Oakes, M. M., Schauer, J. J., Shafer, M. M., Majestic, B. J., and Weber, R. J.: New Technique for Online Measurement of Water-Soluble Fe(II) in Atmospheric Aerosols, *Environ. Sci. Technol.*, 43, 2425–2430, <https://doi.org/10.1021/es8031902>, 2009.
- 825 Rubasinghege, G., Lentz, R. W., Scherer, M. M., and Grassian, V. H.: Simulated atmospheric processing of iron oxyhydroxide minerals at low pH: Roles of particle size and acid anion in iron dissolution, *Proceedings of the National Academy of Sciences*, 107, 6628–6633, <https://doi.org/10.1073/pnas.0910809107>, 2010.
- Salazar, J. R., Pfothenauer, D. J., Leresche, F., Rosario-Ortiz, F. L., Hannigan, M. P., Fakra, S. C., and Majestic, B. J.: Iron Speciation in PM_{2.5} From Urban, Agriculture, and Mixed Environments in Colorado, USA, *Earth and Space Science*, 7, e2020EA001262, <https://doi.org/10.1029/2020EA001262>, 2020a.

- 830 Salazar, J. R., Cartledge, B. T., Haynes, J. P., York-Marini, R., Robinson, A. L., Drozd, G. T., Goldstein, A. H., Fakra, S. C., and Majestic, B. J.: Water-soluble iron emitted from vehicle exhaust is linked to primary speciated organic compounds, *Atmospheric Chemistry and Physics*, 20, 1849–1860, <https://doi.org/10.5194/acp-20-1849-2020>, 2020b.
- Shao, Y., Wyrwoll, K.-H., Chappell, A., Huang, J., Lin, Z., McTainsh, G. H., Mikami, M., Tanaka, T. Y., Wang, X., and Yoon, S.: Dust cycle: An emerging core theme in Earth system science, *Aeolian Research*, 2, 181–204, 835 <https://doi.org/10.1016/j.aeolia.2011.02.001>, 2011.
- Shi, Z., Krom, M. D., Jickells, T. D., Bonneville, S., Carslaw, K. S., Mihalopoulos, N., Baker, A. R., and Benning, L. G.: Impacts on iron solubility in the mineral dust by processes in the source region and the atmosphere: A review, *Aeolian Research*, 5, 21–42, <https://doi.org/10.1016/j.aeolia.2012.03.001>, 2012.
- Shi, Z., Krom, M. D., Bonneville, S., and Benning, L. G.: Atmospheric Processing Outside Clouds Increases Soluble Iron in 840 Mineral Dust, *Environ. Sci. Technol.*, 49, 1472–1477, <https://doi.org/10.1021/es504623x>, 2015.
- Sholkovitz, E. R., Sedwick, P. N., and Church, T. M.: Influence of anthropogenic combustion emissions on the deposition of soluble aerosol iron to the ocean: Empirical estimates for island sites in the North Atlantic, *Geochimica et Cosmochimica Acta*, 73, 3981–4003, <https://doi.org/10.1016/j.gca.2009.04.029>, 2009.
- Slikboer, S., Grandy, L., Blair, S. L., Nizkorodov, S. A., Smith, R. W., and Al-Abadleh, H. A.: Formation of Light Absorbing 845 Soluble Secondary Organics and Insoluble Polymeric Particles from the Dark Reaction of Catechol and Guaiacol with Fe(III), *Environ. Sci. Technol.*, 49, 7793–7801, <https://doi.org/10.1021/acs.est.5b01032>, 2015.
- Sorooshian, A., Brechtel, F. J., Ma, Y., Weber, R. J., Corless, A., Flagan, R. C., and Seinfeld, J. H.: Modeling and Characterization of a Particle-into-Liquid Sampler (PILS), *Aerosol Science and Technology*, 40, 396–409, <https://doi.org/10.1080/02786820600632282>, 2006.
- 850 Stieger, B., Spindler, G., Fahlbusch, B., Müller, K., Grüner, A., Poulain, L., Thöni, L., Seitler, E., Wallasch, M., and Herrmann, H.: Measurements of PM₁₀ ions and trace gases with the online system MARGA at the research station Melpitz in Germany – A five-year study, *J Atmos Chem*, 75, 33–70, <https://doi.org/10.1007/s10874-017-9361-0>, 2018.
- Stieger, B., Spindler, G., van Pinxteren, D., Grüner, A., Wallasch, M., and Herrmann, H.: Development of an online-coupled 855 MARGA upgrade for the 2 h interval quantification of low-molecular-weight organic acids in the gas and particle phases, *Atmospheric Measurement Techniques*, 12, 281–298, <https://doi.org/10.5194/amt-12-281-2019>, 2019.
- Stookey, L. L.: Ferrozine---a new spectrophotometric reagent for iron, *Anal. Chem.*, 42, 779–781, <https://doi.org/10.1021/ac60289a016>, 1970.
- Tang, M., Perron, M. M. G., Baker, A. R., Li, R., Bowie, A. R., Buck, C. S., Kumar, A., Shelley, R., Ussher, S. J., Clough, R., Meyerink, S., Panda, P. P., Townsend, A. T., and Wyatt, N.: Measurement of soluble aerosol trace elements: inter-laboratory 860 comparison of eight leaching protocols, *Atmospheric Measurement Techniques*, 18, 6125–6141, <https://doi.org/10.5194/amt-18-6125-2025>, 2025.
- Teixeira, L. S. G. and Rocha, F. R. P.: A green analytical procedure for sensitive and selective determination of iron in water samples by flow-injection solid-phase spectrophotometry, *Talanta*, 71, 1507–1511, <https://doi.org/10.1016/j.talanta.2006.07.025>, 2007.
- 865 Tilgner, A. and Herrmann, H.: Tropospheric Aqueous-Phase OH Oxidation Chemistry: Current Understanding, Uptake of Highly Oxidized Organics and Its Effects, in: *Multiphase Environmental Chemistry in the Atmosphere*, vol. 1299, American Chemical Society, 49–85, <https://doi.org/10.1021/bk-2018-1299.ch004>, 2018.

- 870 Tsimpidi, A. P., Scholz, S. M. C., Milousis, A., Mihalopoulos, N., and Karydis, V. A.: Aerosol composition trends during 2000–2020: in-depth insights from model predictions and multiple worldwide near-surface observation datasets, *Atmos. Chem. Phys.*, 25, 10183–10213, <https://doi.org/10.5194/acp-25-10183-2025>, 2025.
- Valavanidis, A., Salika, A., and Theodoropoulou, A.: Generation of hydroxyl radicals by urban suspended particulate air matter. The role of iron ions, *Atmospheric Environment*, 34, 2379–2386, [https://doi.org/10.1016/S1352-2310\(99\)00435-5](https://doi.org/10.1016/S1352-2310(99)00435-5), 2000.
- 875 Wang, X., Shen, Z., Huang, S., Che, H., Zhang, L., Lei, Y., Sun, J., Shen, G., Xu, H., and Cao, J.: Water-soluble iron in PM_{2.5} in winter over six Chinese megacities: Distributions, sources, and environmental implications, *Environmental Pollution*, 314, 120329, <https://doi.org/10.1016/j.envpol.2022.120329>, 2022.
- Weber, R. J., Orsini, D., Daun, Y., Lee, Y.-N., Klotz, P. J., and Brechtel, F.: A Particle-into-Liquid Collector for Rapid Measurement of Aerosol Bulk Chemical Composition, *Aerosol Science and Technology*, 35, 718–727, <https://doi.org/10.1080/02786820152546761>, 2001.
- 880 Wong, J. P. S., Yang, Y., Fang, T., Mulholland, J. A., Russell, A. G., Ebel, S., Nenes, A., and Weber, R. J.: Fine Particle Iron in Soils and Road Dust Is Modulated by Coal-Fired Power Plant Sulfur, *Environ. Sci. Technol.*, 54, 7088–7096, <https://doi.org/10.1021/acs.est.0c00483>, 2020.
- Yang, Y., Gao, D., and Weber, R. J.: A Method for Liquid Spectrophotometric Measurement of Various Forms of Iron and Copper in Ambient Aerosols, <https://doi.org/10.5194/amt-2021-72>, 9 March 2021.
- 885 Ye, D., Klein, M., Mulholland, J. A., Russell, A. G., Weber, R., Edgerton, E. S., Chang, H. H., Sarnat, J. A., Tolbert, P. E., and Ebel, S.: Estimating Acute Cardiovascular Effects of Ambient PM_{2.5} Metals, *Environ Health Perspect*, 126, 027007, <https://doi.org/10.1289/EHP2182>, 2018.
- Zeng, L., Sullivan, A. P., Washenfelder, R. A., Dibb, J., Scheuer, E., Campos, T. L., Katich, J. M., Levin, E., Robinson, M. A., and Weber, R. J.: Assessment of online water-soluble brown carbon measuring systems for aircraft sampling, *Atmospheric Measurement Techniques*, 14, 6357–6378, <https://doi.org/10.5194/amt-14-6357-2021>, 2021.
- 890 Zepp, R. G., Faust, B. C., and Hoigne, J.: Hydroxyl radical formation in aqueous reactions (pH 3–8) of iron(II) with hydrogen peroxide: the photo-Fenton reaction, *Environ. Sci. Technol.*, 26, 313–319, <https://doi.org/10.1021/es00026a011>, 1992.
- Zhang, J.-Z., Kelble, C., and Millero, F. J.: Gas-segmented continuous flow analysis of iron in water with a long liquid waveguide capillary flow cell, *Analytica Chimica Acta*, 438, 49–57, [https://doi.org/10.1016/S0003-2670\(01\)01031-5](https://doi.org/10.1016/S0003-2670(01)01031-5), 2001.

895